





**PROFORMA**  
**RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)**  
**BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: PHC PARATHODU	Name of District: KOTTAYAM
Name of Equipment: Biochemistry Analyzer	Equipment ID & Barcode: 146668 & 0542929
Make: Robonik	Model: Prietest Touch
Serial Number: AT2280814RBK	Warranty details: No warranty
Date of purchase/ Date of manufacture/ Installation Date : 28/07/2015	Present status of the equipment: Fully Damaged
Date of breakdown: 14/11/2024 (Toll free) Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CMC
Action taken: Checked and found out the problem with primary board , filters and flow cell with tubing defective .Enquired the spare with oem	

Recommendations for repair (required service details) : Not recommending for repair.

Cost of spares (specify parts and cost): NA

Percentage value of the cost of spares with respect to Cost of purchase/ Asset Value: NA <i>FOI</i>	Asset Value: 67998/-
---	----------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) : Cyrix service report and end of life letter attached


Reasons for recommending the equipment as RBER : Checked and found out the problem with primary board , filters and flow cell with tubing defective , Machine installed in 28/07/2015 and covered up to 9 + years. Oem declared end of life for this machine So recommending the machine for condemnation as per the tender clause .3.14.2

*Ajmal shajahan* *19/12/24*  
 Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM: *Asset value - 67998 / Cost of spare - End of Life letter attached from OEM. The machine installed in 28/7/2015 and completed 9 years - as per these conditions recommended as RBER -*

Recommended for BER (Yes/ No): <i>Yes</i>	
Date: <i>6/12/24</i>	<i>[Signature]</i> Signature of JC BM (NHM)
Date: <i>19/12/2024</i> Medical Officer (i/c) <i>[Signature]</i>	Signature of Superintendent / <i>A</i>

*Seal*  
**The Medical Officer in-charge**  
**F. H. C. Parathodu**  
**Kottayam District**

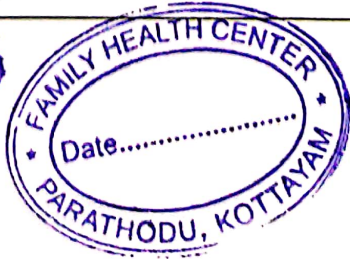




# SEMI AUTO ANALYSER

MAKE : PRIETEST TOUCH  
 MODEL : ROBOTONICS  
 INSTALLATION DATE: 28.09.2015  
 WARRANTY PERIOD : 28.09.2018  
 SERIAL NUMBER : AT 2280814 RBK

## Accessories

- sine wave clips - 1 no
- Halogen lamps - 1 no
- thermal print paper
- Dust covers - 1 no

Cost :- 64760/- + vat 5% = 3238/-  
 serial :- 67998/-

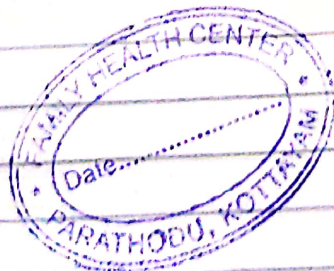


Stmk  
 16/11/24

Forwarded  
 for no  
 [Signature]

19/12/2024  
 The Medical Officer in-charge  
 F. H. C. Parathodu  
 Kottayam District



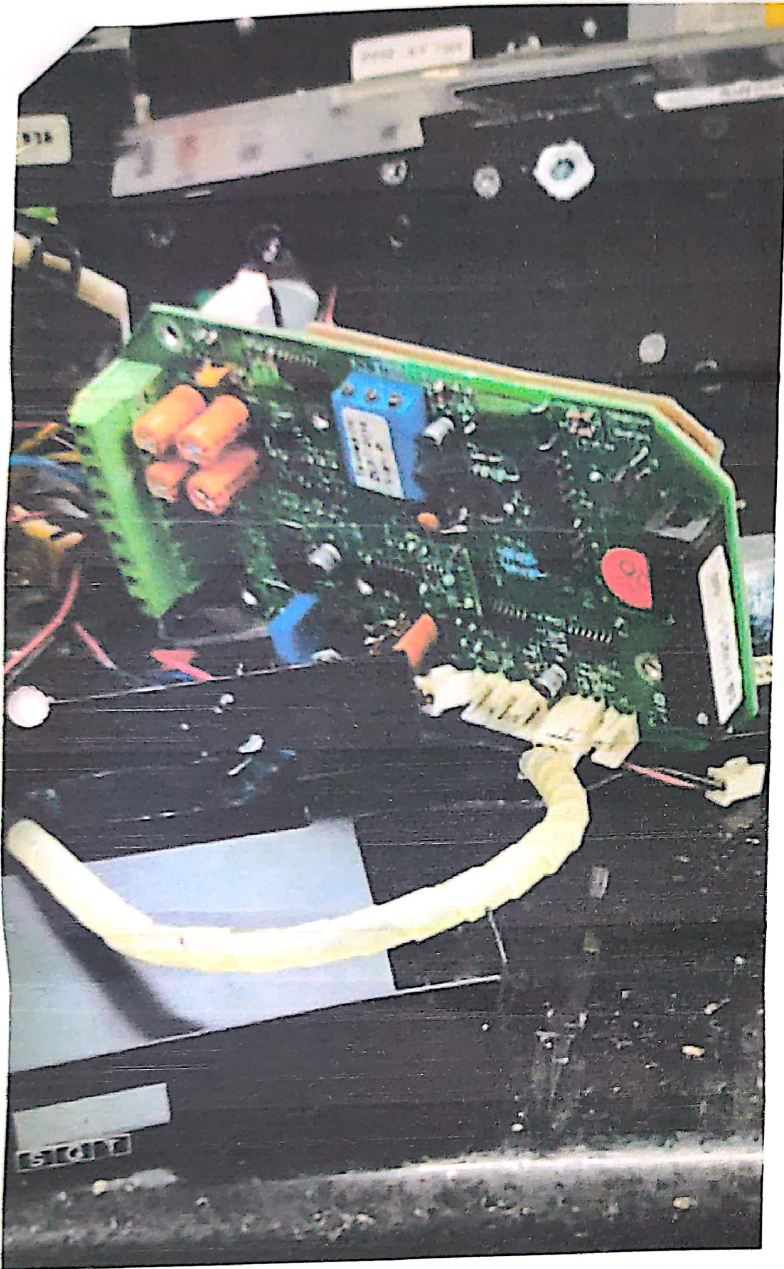

680


**CYRIX** BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)

TOLL FREE NO: 1800 - 425-7669

BAR CODE - (8004-890615225) 0542929



**prn**

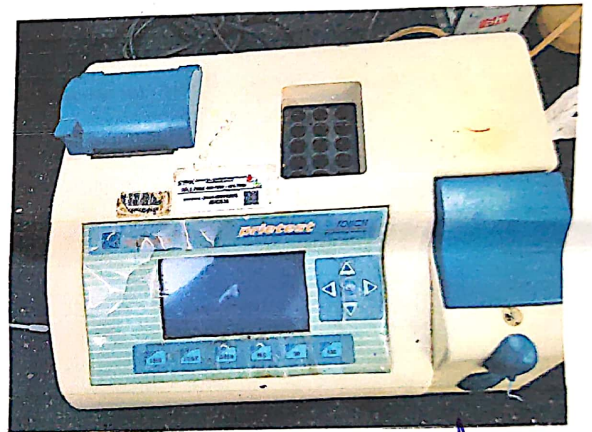

*strik  
12/11/24*

*forwarded  
for me  
19/12/2024*

Model **prietest TOUCH** Voltage 1 **230V 60Hz 50Hz**

Sr. No. **AT2280814RBK** Power **75VA**

Contrast Knob

**CE**

**FAMILY HEALTH CENTRE PARATHODU, KOTTAYAM**

Medical Officer in-charge  
F. H. C. Parathodu  
Kottayam District

**FAMILY HEALTH CENTRE**  
Date.....  
**PARATHODU, KOTTAYAM**



Date: 22.11.2024

Dear Valued Customer,



Thank you for choosing **Robonik (India) Pvt. Ltd.** We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model: Prietest Touch) having Serial No. **AT2280814RBK**.

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having Serial No. **AT2280814RBK** as **End of Life (EOL) Notified.** (During from installation is 10 years).

Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK (INDIA) PVT. LTD.**



Authorised Signatory