



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 133255

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>Thq h Pulinkunnu</u> Address..... <u>Alappuzha</u> Ph:..... <u>9447243792</u>	Call Registration Date :..... <u>11/12/24</u> Caller ID :..... <u>152065</u> Date of Visit :..... <u>12/12/24</u> Asset No :..... <u>042124</u> EQPT Name :..... <u>Nebulizer</u> Manufacture..... <u>OMRON</u> Model :..... <u>Omron</u> S. No..... <u>00167847</u> Dept..... <u>Opd</u>
---	---

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : flame not coming

Action Taken : checked & found that compressor motor with piston Defectiv. need to replace them spare for further checking & starting condition of the equipment.

Completed Date : 12/12/24 Time : 1:30pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrux Engineer	Date	Start Time	End Time
<u>Anandha Krishnan P</u>	<u>12/12/24</u>	<u>12 pm</u>	<u>1:30 pm</u>

Customer Remark Completed Pending

Service Engineer Name : Anandha Krishnan P
Signature: [Signature]
Date: 12/12/24
Contact Number: 994140501

SUPERINTENDENT
 THQ HOSPITAL
Customer Name: recharge OPD
Signature: [Signature]
Date: [Date]
Contact Number: 472492
Designation : SA
Hospital Seal



N.G.BULI 2012

YGA

Store

Rec. - P. (L)

12/15 Received from the Store

7

1

8

21/15 NS per order no 6-1111

1

(2015) T.H.H. Dated 13/11/15
Covolumed

2

1

6

Sub

12/15 Received from the Store

6

1

7

(Nebulizer)

Sub

5/4/17 Received from store

7

2

89

8 (M.S No. 25)

Sub

(Extra care (R))


NS received from store

1

1

10

NS page 25 v 5



For
Superintendent
T.H.H,
Pulincunnu

SUPERINTENDENT
THQ HOSPITAL
PULINCUNNU

28/



25/

20/

20/20

5/10/11

6/10/11

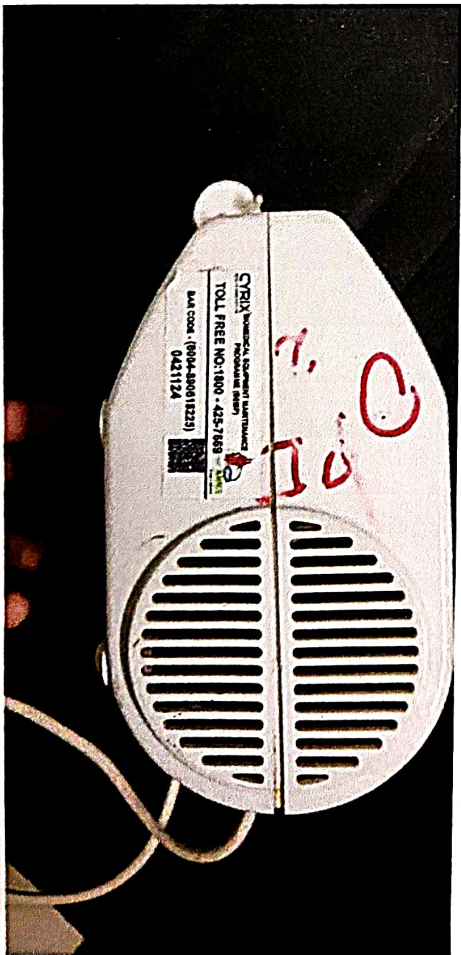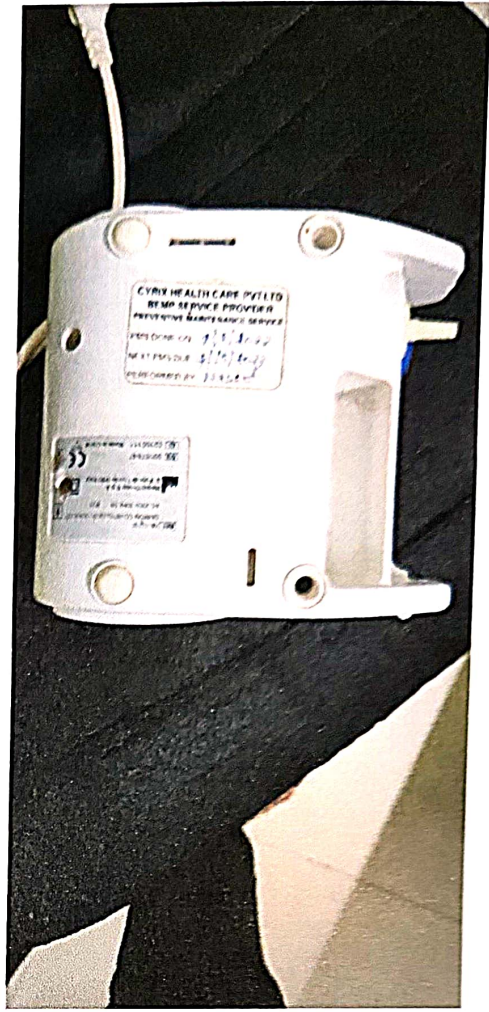


SUPERINTENDENT
THQ HOSPITAL
PULINCUNNU



PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: THQH PULINKUNNU	Name of District: Alappuzha
Name of Equipment: NEBULISER	Equipment ID & Barcode: 152065 & 0421124
Make: OMRON HEALTHCARE CO.LTD.	Model: NA
Serial Number: 00167847	Warranty details: NO WARRANTY
Date of purchase/ Year of manufacture/ Installation Date: 12-05-2016	Present status of the equipment: MACHINE FULLY DAMAGED
Date of breakdown: 11/12/2024 (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: NO AMC/CAMC

Action taken: CHECKED AND FOUND THAT COMPRESSOR MOTOR WITH PISTON DEFECTIVE.NEED TO REPLACE THESE SPARES FOR FURTHER CHECKING AND WORKING CONDITION OF THE EQUIPMENT.


Recommendations for repair (required service details): Not recommended for repair

Cost of spares (specify parts and cost): Not available


# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: Not available	Asset Value: 1353/-
---	---------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)
 Cyrix service report attached


Reasons for recommending the equipment as BER: CHECK AND FOUND THAT COMPRESSOR MOTOR WITH PISTON DEFECTIVE. MACHINE WAS AGED UPTO 8+ YRS AND QUOTATION NOT SUBMITT SINCE SPARES ARE NOT AVAILABLE IN THE MARKET.SO RECOMMENDING THE EQUIPMENT FOR RBER

Anandkavishnan.P  17/12/24
 Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
 Recommended for BER

Recommended for BER (Yes/ No): Yes	JYOTHISH THOMAS Consultant (Biomedical Engineering) NHM ALAPPUZHA  17/12/24 Signature of JC BM (NHM)
Date: 17/12/24	

Date: 17/12/24
 Medical Officer (i/c)




 Signature of Superintendent /

SUPERINTENDENT
THQ HOSPITAL
PULINCUNNU