



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1010683

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website :www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>DH Aluva</u> Address..... <u>Ernakulam</u> Ph:..... <u>9547429749</u>	Call Registration Date : <u>20/6/24</u> Caller ID : <u>118121</u> Date of Visit : <u>21/06/24</u> Asset No : <u>0712037</u> EQPT Name : <u>Blood bank Refrigerator</u> Manufacture..... <u>Lab lin</u> Model : <u>NA</u> S. No. <u>06K-1722</u> : Dept..... <u>Blood bank</u>
---	---

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : Malfunction.....

Action Taken : checked and found compressor, cooling - coil, condenser, Digital controller, condenser, Digital controller, fan motor with blower, Handle and light defective, need these parts for further checking and working condition of the equipment.....

Completed Date : 26/7/24 Time : 1.00 pm Spare Required

Spare Replaced Requested


Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer <u>Alwin</u>	Date <u>26/7/24</u>	Start Time <u>12:30 pm</u>	End Time <u>1:00 pm</u>
--------------------------------	------------------------	-------------------------------	----------------------------

Customer Remark Completed Pending

Pending repair

Service Engineer Name : <u>Alwin</u> Signature: <u>[Signature]</u> Date: <u>26/7/24</u> Contact Number: <u>9745847238</u>	Customer Name : Signature: <u>[Signature]</u> Date: Contact Number: Designation: Hospital Seal
--	---

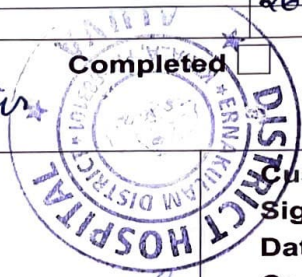

SUPERINTENDENT
DISTRICT HOSPITAL
ALUVA

Dr. N.VIJAYA KUMAR
Medical Officer in charge
Regional Blood Transfusion Centre
District Hospital, Aluva

PEROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: DH Aluva	Name of District: Ernakulam
Name of Equipment: Blood Bank refrigerator	Equipment ID & Barcode: 118121& 0712037
Make: Lab Line	Model: BBR 288
Serial Number: 06K- 1722	Warranty details: NA
Date of purchase/ Year of manufacture/ Installation Date: 11-12-2006	Present status of the equipment: Not Working
Date of breakdown: 20-06-2024 (Toll Free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: NA

Action taken: Checked and found compressor, cooling coil, condenser, digital controller, fan motor with blower, handle and light defective. Need gas charging also. Need to replace these spares for further checking and working condition of the equipment.

Recommendations for repair (required service details): Not recommending for repair

Cost of spares (specify parts and cost): Compressor-23010, Cooling coil-10030, Condenser-7670, Digital controller-6750, Fan motor with blower-12980, Handle-531, Light-620, Gas charging-16520
 Total-Rs-93486

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 133%	Asset Value: 70000/-
--	----------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
 Cyrix Service report and OEM Quotation attached.

Reasons for recommending the equipment as BER: Checked and found compressor, cooling coil, condenser, digital controller, fan motor with blower, handle and light defective. Need gas charging also. Machine installed on 11-12-2006 and covered up to 17+ years. Repairing cost of the equipment is 133%, both criteria met. So recommending the equipment for condemnation as per tender clause 5.3.14.1.

ALWIN PETER

Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM: Multiple spare damage reported by Cyrix. Equipment installed in 2006 and met yearwise BER criteria. Quot attached. Stock attached without seal. Recently repaired and replace parts more than 2 time. Submitted after 30 days. Yearwise and date wise criteria met. Final recommendation up to KMSCL.

Recommended for BER (Yes/ No): Decision up to KMSCL

Date: 29/11/24.

CONSULTANT
 Bio-Medical Engineer
 National Health Mission (NHM)
 Aroyyakeralam Ernakulam

Signature of JC BM (NHM)
 29/11/24

Date:
 Medical Officer (i/c)



Signature of Superintendent /

SUPERINTENDENT
DISTRICT HOSPITAL
ALUVA

3 ✓	BLOOD BANK REFRIGERATOR	LABLING	BBR 288 CGK-0722	11-12-2006	03
4 ✓	BLOOD BANK REFRIGERATOR	LABLING			



Signature

**SUPERINTENDENT
DISTRICT HOSPITAL
ALUVA**

LABLINE INSTRUMENTS
ISO 9001:2015 CERTIFIED

Opp KWA Azad Junction, Eroor South, Tripunithura- 682306 TEL : 9496679174
EMAIL:lablinefactories@gmail.com

Ref No: LF/60/2024-25
23-07-2024

Cyrix Health Care Pvt Ltd
Poonithura, Cochin

Our Engineer has inspected the defective instruments and we are pleased to submit our repair estimate as given below.

1. Item Name: Blood Bank Refrigerator BBR288 06 K 1722

Sl. No.	Product details	Estimated Cost	Qty	GST@18%	Amount
1	Compressor	19500.00	1 No	3510.00	23010.00
2	Cooling Coil	8500.00	1 No	1530.00	10030.00
3	Condenser	6500.00	1 No	1170.00	7670.00
4	Digital Controller	6750.00	1 No	1215.00	7965.00
5	Fan Motor with blower	11000.00	1 No	1980.00	12980.00
6	Handle	450.00	1 No	81.00	531.00
7	Light	525.00	1 No	95.00	620.00
8	Gas Charging	14000.00	1 No	2520.00	16520.00
9	Service Charge	12000.00	1 No	2160.00	14160.00
		79225.00		TOTAL	93486.00

Note: After replacing the above spare and any of the parts has been found defective a new estimate will be given

TERMS AND CONDITIONS

GST : Inclusive
Validity : 30 Days
Payment : 100% advance

Thanking you,
FOR LABLINE INSTRUMENTS



SUPERINTENDENT
DISTRICT HOSPITAL
ALUVA



Fw: Estimate

From DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>
Date Wed 2024-10-09 05:28 PM
To faizalscyrix@gmail.com <faizalscyrix@gmail.com>
Cc Afsal Yunuze <zm1.klbemp@cyrix.in>

📎 1 attachment (2 MB)
Cyrix BBR.pdf;

DH ALUVA - BBR QUOTATION


Thanks & Regards,
Abijith.A
Divisional Manager | South Zone
dm2.klbemp@cyrix.in
www.cyrixhealthcare.com
Cyrix Healthcare Pvt Ltd
| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India
KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH

From: Labline Instruments <lablinefactories@gmail.com>
Sent: 26 July 2024 11:19 AM
To: DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>
Subject: Estimate

Dear Sir,

Please find the attached estimate

--
Regards,
VISHNU
Labline Factory



[Handwritten Signature]
**SUPERINTENDENT
DISTRICT HOSPITAL
ALUVA**



MODEL No. BBR-2555 SL. No. 06K-1799
WATTS 3000 WATTS 220/230V AC 1 ϕ 50Hz
LABLINE INSTRUMENTS
COCHIN, INDIA-682 301



[Handwritten signature]

**DISTRICT HOSPITAL
ALUVA**

[Handwritten signature]
**SUPERINTENDENT
DISTRICT HOSPITAL
ALUVA**