



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 135363

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website :www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>CHC</u> Address..... <u>puthen shoppu</u> <u>Thiruvananthapuram</u> Ph:..... <u>9946368905</u>	Call Registration Date :..... <u>6/11/24</u> Caller ID :..... <u>145161</u> Date of Visit :..... <u>6/11/24</u> Asset No :..... <u>0130288</u> EQPT Name :..... <u>UPS</u> Manufacture..... <u>V Guard</u> Model : <u>NA</u> S. No..... <u>NA</u> Dept..... <u>Lab</u>
---	--

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : NOT WORKING

Action Taken : Checked and found that the inverted PCB, Control PCB and 12V 7AH battery defective. Need to Replace these spares for further checking and working condition of the equipment. Enquired spare with vendor.

Completed Date : 6/11/24 Time :..... 12 PM Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Deepak</u>	<u>6/11/24</u>	<u>11:30</u>	<u>12 PM</u>

Customer Remark : Completed Pending

Service Engineer Name : <u>Deepak</u> Signature: <u>[Signature]</u> Date: <u>6/11/24</u> Contact Number: <u>7902991038</u>	Customer Name: <u>[Signature]</u> Signature: <u>[Signature]</u> Date: <u>6/11/24</u> Contact Number: <u>9946368905</u> Designation : <u>[Signature]</u> Hospital Seal: <u>[Signature]</u>
---	--

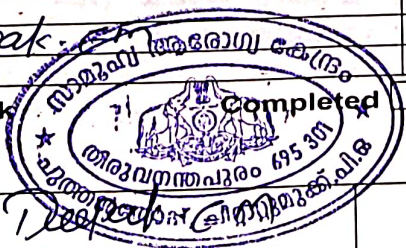

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC PUTHENTHOPPE	Name of District: Thiruvananthapuram
Name of Equipment: UPS	Equipment ID & Barcode: 145161 & 0130288
Make: V GUARD	Model: 1 KV
Serial Number : NA	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 01/09/2018	Present status of the equipment: Fully Damaged
Date of breakdown: 06/11/2024(Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC

Action taken: Checked and found that the inverter PCB and 12v 7Ah battery defective. Need to replace these spares for further checking and working condition of the equipment. Enquired spare with vendor

Recommendations for repair (required service details) : Not recommending for repair.

Cost of spares (specify parts and cost) :
 1. 1KVA 24V Inverter PCB - 4130/-
 2. 12v 7 Ah Battery (2Nos) - 2176/-
 Total = 6306/-

Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 140.1% Asset Value: 4500/-

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
Cyrix service report and reference quotation attached.

Reasons for recommending the equipment as BER: Checked and found that the inverter PCB and 12v 7Ah battery defective. The unit was installed on 01/09/2018 and covered up to 6+ years. The repairing cost is 140.1%. As per the tender clause 5.3.14.1 Both criteria met. So recommending the unit for condemnation.

Kasyep.pv *[Signature]*
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
*Spare value is more than asset value since the value is normalised for UPS.
 So KMSCL can take decision in this case.*

Recommended for BER (Yes/ No):

Date:



Date:

[Signature]
MANEESHA MOHAN M.R.
 Junior Consultant (Biomedical)
 National Health Mission
 Thiruvananthapuram
 Superintendent's Office (i/c)
 കാമുകി സർവ്വകലാശാല, ചിറ്റാറ്റുപുഴ, തിരുവനന്തപുരം 695 301

FULLY AUTOMATIC HAEMATOLOGY ANALYZER

8/2/16

with full expert
Key Board mode.
Haematology Analyzer
Serial: 20151100056285
(Consul Newall) Rapid Diagnostics
Accuracy period - 2 years
8/12/16 to 8/12/19
UPS complete on - 8/9/18
New ups - provision installed on - 13/9/18
(Calibration)

model - 21101
- 11101
Capacity - 9,000 test (12-1000)
Out put - Input - 220/100/50 Hz
- 6000 - 220V 50/60 Hz
Code: - 11102117000123
1048
Bm. cust - 70010454
- SN. No. P222117000636

130

Rt Clock - function - Serial
P2 clock - function - Serial



Calibration
Calibration

Signature

2.
23-11-20

LAB X (Supplier Name)
Machine - Medonic M Series M32B
Invoice No - EC/1788
Dated - 23-NOV-2020
Buyers Order No - C-368/2020/CHCP
Dated - 6-NOV-2020

₹ 1,71,360
(Invoice No. EC/1788)
Registered Agents: 63 Store

1. Medonic M series, M 32B
2. Medonic M series Diluent, RFID 20L (50446)
3. Medonic M series Lyse, RFID 5L (50446)
4. Green Bio 900/12v with 2 Nos 7 AH Battery
5. Printer Epson LX310 Dotmatrix B

Batch 114853 = ₹ 1,44,000.
Batch 2006-353 Exp 8/6/20
Batch 2005-341 Exp 3/5/2020
Batch 201004586
Batch Q7DY10A844

Total = ₹ 1,71,360.00
Installation ; Warr-4/3/24

AION BACKUPS

YP/VIII/320 AYLARA, KERALA KOLLAM

Date: 13/07/2024

Contact: 8921950217

Email: aionbackups12@gmail.com

GSTIN : 32CGUPM9450L1ZN

1KVA ONLINE UPS SERVICE PROPOSAL

TO,
CYRIX HEALTHCARE PVT. LTD
Barcode: 0130192
Ticket ID: 113214

Dear Sir/Madam,

We are pleased to submit here with our quote for the same as per below.

SL	DESCRIPTION	QTY	UNIT RATE IN INR	TOTAL	GST	TOTAL PRICE IN INR
1	1KVA 24V INVERTER PCB	1	3500.00	3500.00	18	4130.00
2	1KVA CONTROL PCB	1	2500.00	2500.00	18	2950.00
3	12v 7Ah Battery	2	850.00	1700.00	28	2176.00
PAYABLE AMOUNT						9256.00
Commercial terms and conditions 1. Payment 80% advance along with PO balance before dispatch, 20%After installation. 2. Delivery period; 2weeks. 3. Tax :GST@18% for spares, 28%@Battery 4. Installation; Our scope.						
Please arrange to release the PO at our above address						
Bank name :HDFC		Account no:50200082743176		IFSC Code:HDFC0004083		
We hope you will find the above offer in line with our discussions and await your valuable order please free to call or mail us on above given number if any query. Thank you, Sincerely, BHAGATH MOHAN						





REGARDING QUOTATION FOR UPS-CHC ANCHUTENGU (0130192 0130178)

2 messages

Kasyep P V <kasyepcyrix@gmail.com>

Thu, 18 Jul 2024 at 10:02 pm

To: aionbackups12@gmail.com <aionbackups12@gmail.com>

Dear sir,

Kindly provide the service quotation for the 1 KV UPS at CHC Anchuthengu, Trivandrum

--

Thanks & Regards,

KASYEP PV

District Incharge , Trivandrum

CYRIX HEALTHCARE Pvt.Ltd

KLBEMP

Ph : +91 7593847134

kasyepcyrix@gmail.com

Bhagath Mohan <aionbackups12@gmail.com>

Thu, 18 Jul 2024 at 11:19 pm

To: Kasyep P V <kasyepcyrix@gmail.com>


Received your mail.

Thanks & Regards

Bhagath Mohan

PH:-8921950217

[Quoted text hidden]

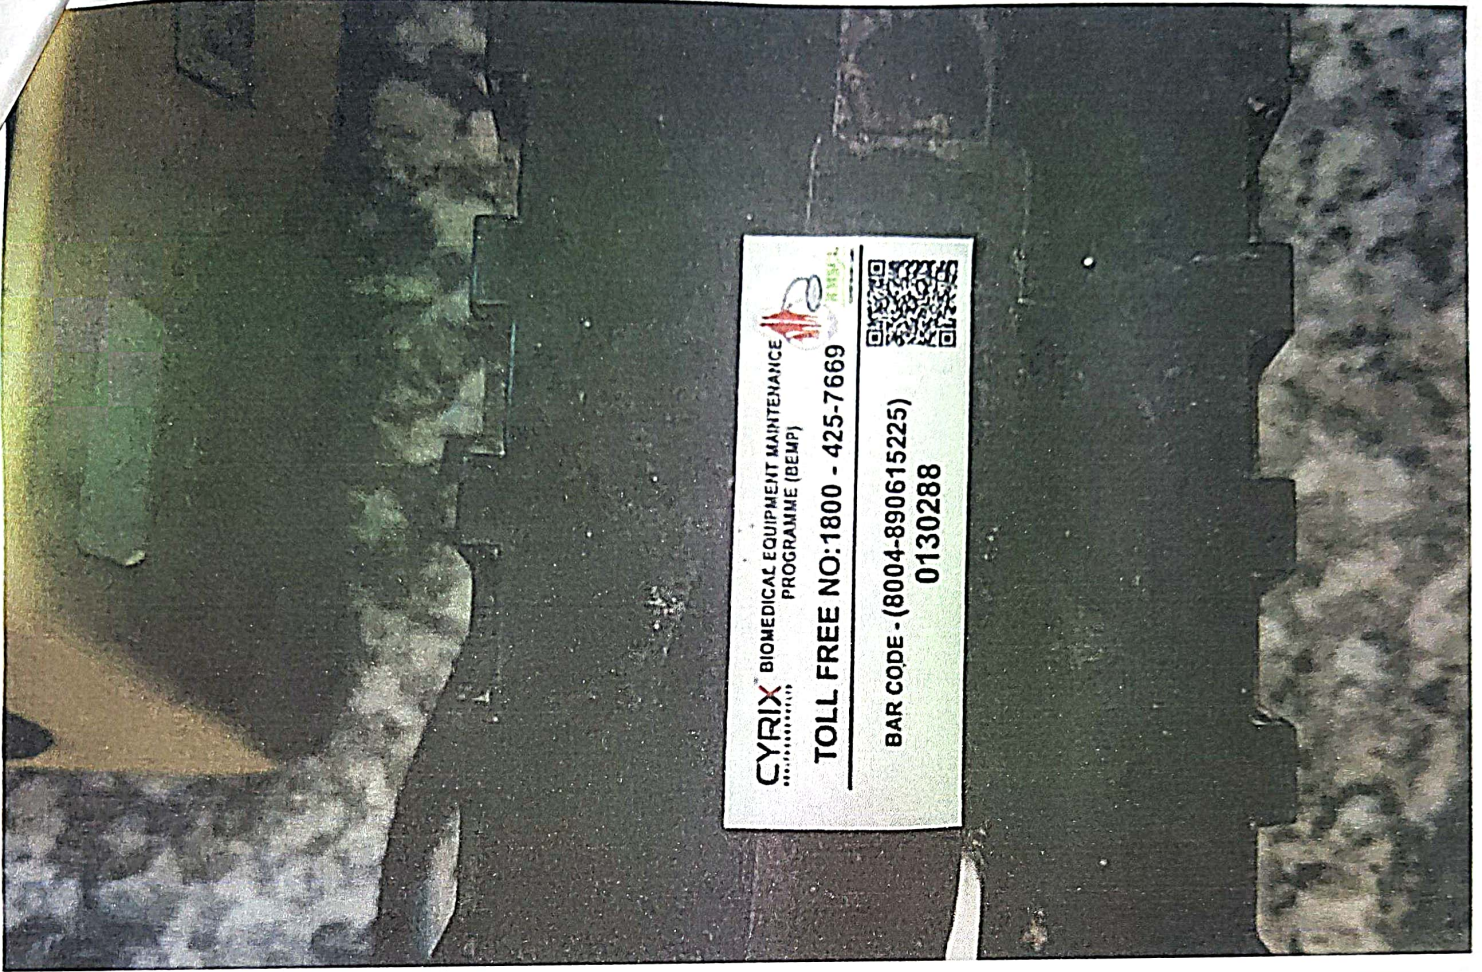

ശ്രീ. [Signature]
 ഡയറക്ടർ, കേരള ആരോഗ്യ സൗകര്യ വകുപ്പ്, തിരുവനന്തപുരം 695 301