



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 135362

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>CHC</u>	Call Registration Date : ... <u>6/11/24</u>
Address..... <u>Puthen Shoppu</u>	Caller ID : ... <u>145117</u>
<u>Thiruvananthapuram</u>	Date of Visit : ... <u>6/11/24</u>
Ph: ... <u>9946368905</u>	Asset No : ... <u>0130289</u>
	EQPT Name : ... <u>UPS</u>
	Manufacture... <u>V.Guard</u> Model : ... <u>NA</u>
	S. No..... <u>NA</u> Dept. <u>Lab</u>

Service Classification : Breakdown call PMS Calibration Cust. Training


Problem Identified : ... Not working

Action Taken : ... Checked and found that the inverted PCB, Control PCB and 12V 7AH Battery defective. Need to Replace these spares for further checking and working condition of the equipment. Enquired spare with vendor.

Completed Date : 6/11/24 Time : ... 11:30am Spare Required

Spare Replaced Requested

Description	Qty	Part Number	PR Number
1.			
2.			
3.			

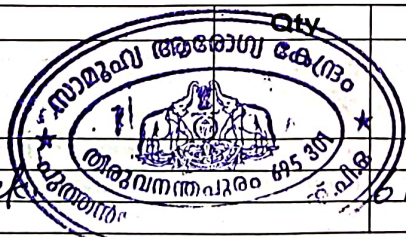

Cyrix Engineer	Date	Start Time	End Time
<u>Deepak</u>	<u>6/11/24</u>	<u>11am</u>	<u>11:30</u>

Customer Remark Completed Pending

Service Engineer Name : Deepak.em
Signature: [Signature]
Date: 6/11/24
Contact Number: 7902881038

Customer Name: [Signature]
Signature: [Signature]
Date: 6/11/24
Contact Number: 9946368905
Designation : [Signature]
Hospital Seal: [Signature]

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC PUTHENTHOPPE	Name of District: Thiruvananthapuram
Name of Equipment: UPS	Equipment ID & Barcode: 145117 & 0130289
Make: V GUARD	Model: Slender Plus 600
Serial Number : NA	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 22/06/2019	Present status of the equipment: Fully Damaged
Date of breakdown: 06/11/2024(Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC

Action taken: Checked and found that the inverter PCB and 12v 7Ah battery defective. Need to replace these spares for further checking and working condition of the equipment. Enquired spare with vendor

Recommendations for repair (required service details) : Not recommending for repair.

Cost of spares (specify parts and cost) :

- 1KVA 24V Inverter PCB - 1475/-
- 12v 7 Ah Battery (2Nos) - 1408/-
- Transformer - 1121/-

Total = 4004/-

# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 88.9%	Asset Value: 4500/-
---	---------------------



Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
Cyrix service report and reference quotation attached.

Reasons for recommending the equipment as BER: Checked and found that the inverter PCB and 12v 7Ah battery defective. The unit was installed on 22/06/2019 and covered up to 5+ years. The repairing cost is 88.9%. As per the tender clause 5.3.14.1 Both criteria met. So recommending the unit for condemnation.

Kasyep.p.v
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
Spare value is high . so it can be RBER and further decision can be taken by kmseL

Recommended for BER (Yes/ No):	 MANEESHA MOHAN M.R. Junior Consultant (Biomedical) National Health Mission Thiruvananthapuram Signature of JC BM (NHM)
Date:	

Date:	 Seal	 Signature of Medical Officer (i/c)
-------	---	--

മെഡിക്കൽ ഓഫീസർ (i/c)
 സാമൂഹ്യ ആരോഗ്യ മിഷൻ
 പുത്തന്തോളം, ചിറ്റാറ്റുരുക്ക്, പി.എ.
 തിരുവനന്തപുരം 695 301

AION BACKUPS

YP/VIII/320 AYLARA, KERALA KOLLAM

Date: 05-09-2024

Contact: 8921950217

Email: aionbackups12@gmail.com

GSTIN: 32CGUPM9450L1ZN

APC 600VA UPS SERVICE PROPOSAL

TO,

CYRIX HEALTHCARE PVT. LTD

Barcode: 130483 – Ticket: 131514

Dear Sir/Madam,

We are pleased to submit here with our quote for the same as per below.

SL	DESCRIPTION	QTY	UNIT RATE IN INR	TOTAL	GST%	TOTAL PRICE IN INR
1	12V INVERTERPCB	1	1250.00	1250.00	18	1475.00
2	12V 7Ah SMF BATTERY	1	1100.00	1100.00	28	1408.00
3	TRANSFORMER	1	950.00	950.00	18	1121.00
PAYABLE AMOUNT						4004.00

Commercial terms and conditions

1. Payment 80% advance along with PO balance before dispatch, 20% after installation.
2. Delivery period; 2weeks.
3. Tax :GST@18% for spares,28%@Battery
4. Installation; Our scope.

Please arrange to release the PO at our above address

Bank name :HDFC

Account no:50200082743176

IFSC Code:HDFC0004083

We hope you will find the above offer in line with our discussions and await your valuable order please free to call or mail us on above given number If any query.

Thank you,

Sincerely,

BHAGATHMOHAN





REGARDING QUOTATION FOR UPS-CHC ANCHUTENGU (0130192 0130178)

2 messages

Kasyep P V <kasyepcyrix@gmail.com>

Thu, 18 Jul 2024 at 10:02 pm

To: aionbackups12@gmail.com <aionbackups12@gmail.com>

Dear sir,

Kindly provide the service quotation for the 1 KV UPS at CHC Anchuthengu, Trivandrum

--

Thanks & Regards,

KASYEP PV

District Incharge , Trivandrum

CYRIX HEALTHCARE Pvt.Ltd

KLBEMP

Ph : +91 7593847134

kasyepcyrix@gmail.com

Bhagath Mohan <aionbackups12@gmail.com>

Thu, 18 Jul 2024 at 11:19 pm

To: Kasyep P V <kasyepcyrix@gmail.com>




Received your mail.

Thanks & Regards

Bhagath Mohan

PH:-8921950217

[Quoted text hidden]

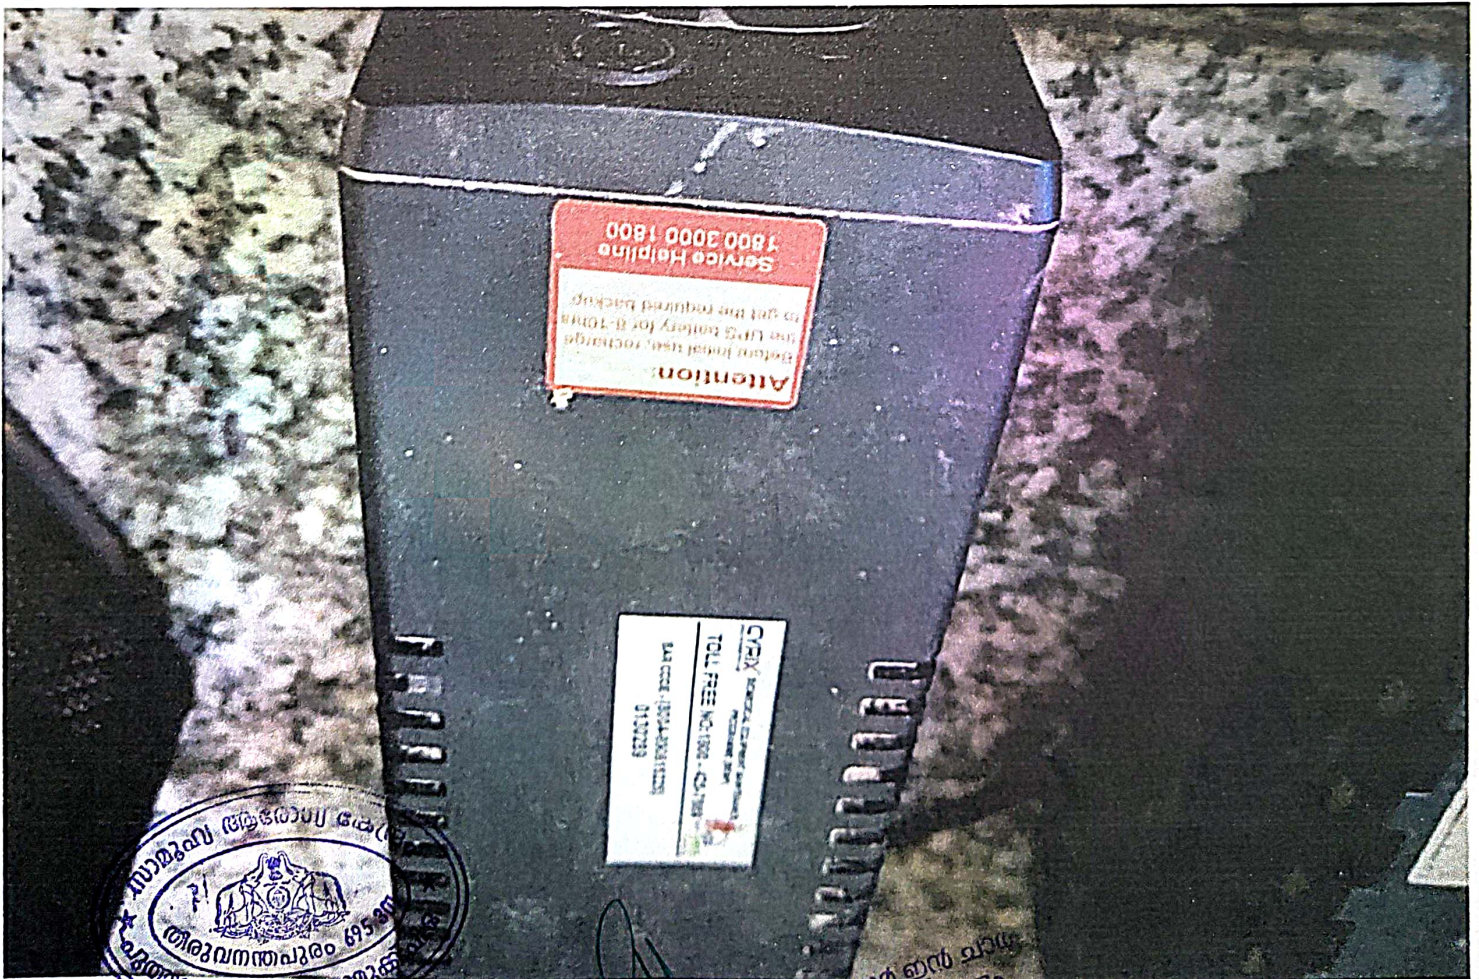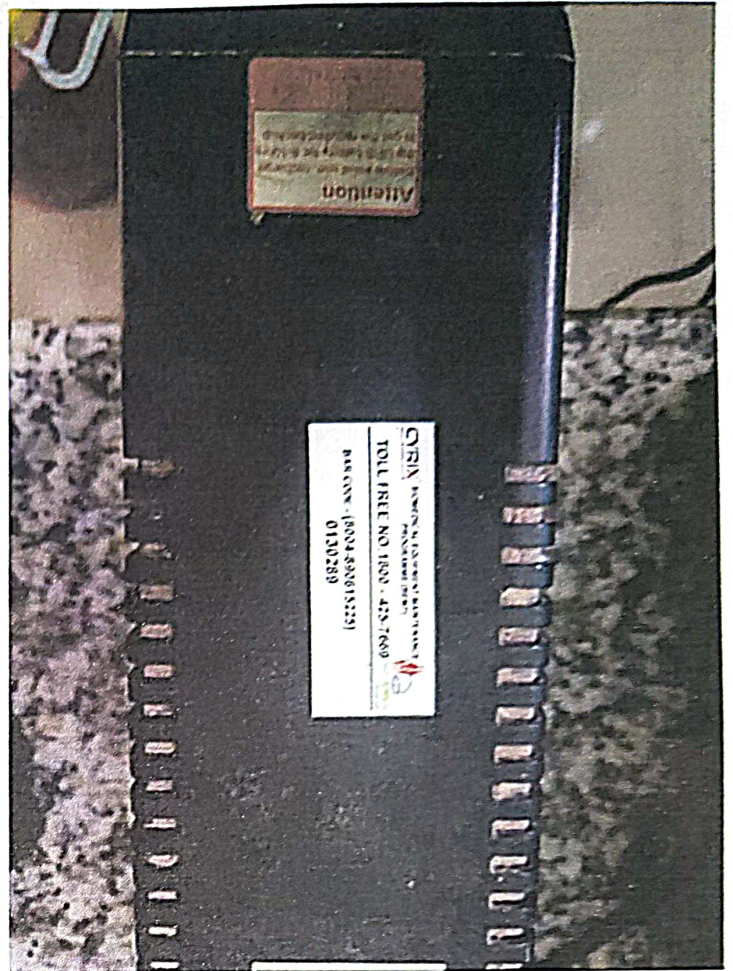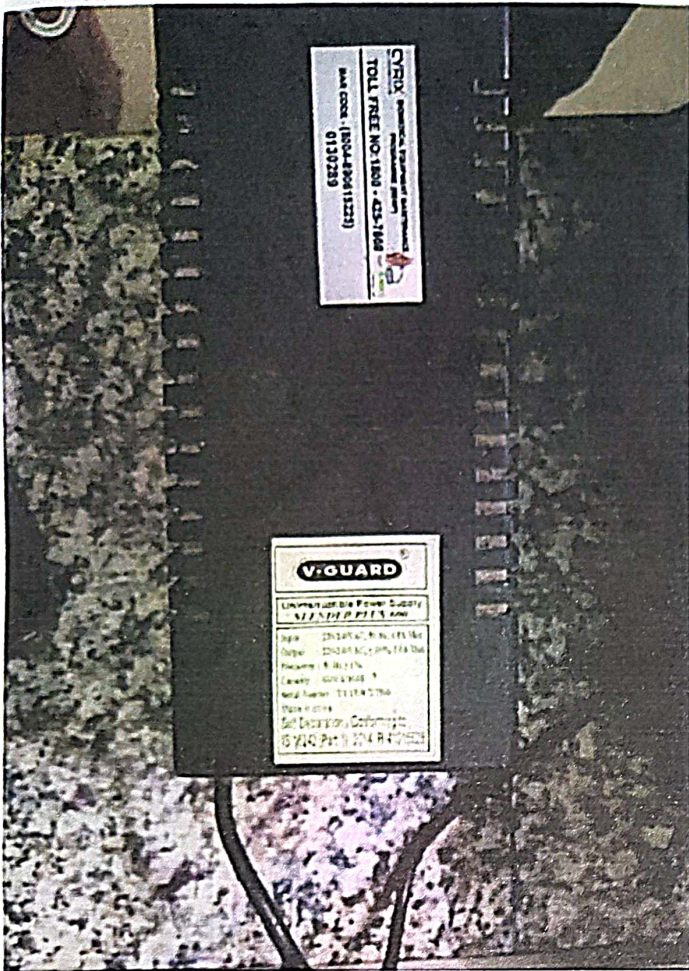

കേരള സംസ്ഥാന വൈദ്യുത വിതരണ കമ്മീഷൻ
 തിരുവനന്തപുരം
 695 301

കൃഷ്ണകുമാർ ആയിരപ്പൻ
 സാമൂഹ്യ ആരോഗ്യ കേന്ദ്രം
 പുത്തത്തോപ്പ്, ചിറ്റാറ്റുരുക്ക്, പി.ഒ.
 തിരുവനന്തപുരം 695 301