



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 135361

CYRIX®

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>CHC</u>	Call Registration Date : .. <u>6/11/24</u>
Address..... <u>Puthen Shoppu</u>	Caller ID : .. <u>145114</u>
<u>Thiruvananthapuram</u>	Date of Visit : .. <u>6/11/24</u>
Ph : .. <u>9946368905</u>	Asset No : .. <u>0130291</u>
	EQPT Name : .. <u>UPS</u>
	Manufacture .. <u>power ups</u> Model : .. <u>APC</u>
	S. No. <u>NA</u> Dept. <u>Lab</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : .. Not working

Action Taken : .. checked and found that the PCB and 12V 7AH Battery defective. Need to Replace these spares for further checking and working condition of the equipment. Enquired spare with vendor

Completed Date : .. 6/11/24 Time : .. 11am Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Deepak</u>	<u>6/11/24</u>	<u>10.30</u>	<u>11 am</u>

Customer Remark : .. Completed Pending

Service Engineer Name : .. Deepak
Signature: [Signature]
Date: 6/11/24
Contact Number: 7902881038

Customer Name: .. [Signature]
Signature: [Signature]
Date: 6/11/24
Contact Number: 9946368905
Designation : .. [Signature]
Hospital Seal: [Signature]



PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: CHC PUTHENTHOPPE	Name of District: Thiruvananthapuram
Name of Equipment: UPS	Equipment ID & Barcode: 145114 & 0130291
Make: APC	Model: BACKUP UPS -600
Serial Number : NA	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 07/03/2017	Present status of the equipment: Fully Damaged
Date of breakdown: 06/11/2024(Toll free) (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC

Action taken: Checked and found that the inverter PCB, Control PCB and 12v 7Ah battery defective. Need to replace these spares for further checking and working condition of the equipment. Enquired spare with vendor

Recommendations for repair (required service details) : Not recommending for repair.

Cost of spares (specify parts and cost) :
 1. 1KVA 24V Inverter PCB - 4130/-
 2. 12v 7 Ah Battery (2Nos) - 2176/-
 Total = 6306/-

Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 140.1% Asset Value: 4500/-

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not):
Cyrix service report and reference quotation attached.

Reasons for recommending the equipment as BER: Checked and found that the inverter PCB, Control PCB and 12v 7Ah battery defective. The unit was installed on 07/03/2017 and covered up to 7+ years. The repairing cost is 140.1%. As per the tender clause 5.3.14.1 Both criteria met. So recommending the unit for condemnation.

Kasyep-p-v Kimsyep
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:

Repair cost is more than asset value. Submitted on 16-12-2024
So can be RBER as per guidelines.
KMSCL can take necessary action directions if needed. *Subo*

Recommended for BER (Yes/ No):

Date: 16-12-2024

MANEESHA MOHAN M.F.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram

Date:



Seal

Signature of Superintendent Medical Officer (i/c)

[Signature]
 ഹെഡ് ക്വട്ടർ സൂപ്രണ്ട് മെഡിക്കൽ ഓഫീസർ (i/c)
 നാഷണൽ ആരോഗ്യ കേന്ദ്രം
 പുത്തൻതോപ്പ്, ചിറ്റാറ്റുരുക്ക്, പി.ഒ.
 തിരുവനന്തപുരം 695 301


SEMI ANALYSER

Date	Recpt.	Blnc.	Company of Blch. No.
15.6.22	✓	1	A Teo 2042 RBk. Supplied by KMSCL through Robnic, India Pvt Ltd. Rs. 24,950/-
	1	1	Halogen Lamp
	2		Thermal print paper
	1	1	Dust Cover.
	1	1	Sight wave UPS. (Sundar) 70010452 (Sundar)
7/03/17	01	02	MISPA VIVA - 21130100 70010452 Supplied by KMSCL, through Agapre. Accessories... 4000 and over Thermal print paper 70010452 UPS 70010452
22/6/19	01	03	Robnic - prietest - Touch semi auto Analyser. Issued from Govt Hospital Twpm. UPS

Bill Invoice - NO: 153
 Bill date - 1.12.19
 Supplied KMSCL.

Barcode - 69014133

Clinical over to Unverifiable registers
 Robnic prietest 69014133 - Nos - 29/10/21

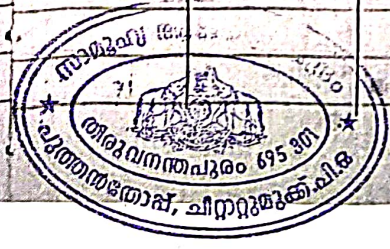

[Handwritten Signature]

മെഡിക്കൽ ഓഫീസർ ഇൻ ചാർജ്
 സാമൂഹ്യ ആരോഗ്യ കേന്ദ്രം
 പുത്തൻതോപ്പ്, ചിറ്റൂർ ജില്ല
 തിരുവനന്തപുരം 695 301



YP/VIII/320 AYLARA, KERALA KOLLAM

Date: 13/07/2024

Contact: 8921950217

Email: aionbackups17@gmail.com

GSTIN : 32CGUPM9450L1ZN

1KVA ONLINE UPS SERVICE PROPOSAL

TO,
CYRIX HEALTHCARE PVT. LTD
Barcode: 0130192
Ticket ID: 113214

Dear Sir/Madam,

We are pleased to submit here with our quote for the same as per below.

SL	DESCRIPTION	QTY	UNIT RATE IN INR	TOTAL	GST	TOTAL PRICE IN INR
1	1KVA 24V INVERTER PCB	1	3500.00	3500.00	18	4130.00
2	1KVA CONTROL PCB	1	2500.00	2500.00	18	2950.00
3	12v 7Ah Battery	2	850.00	1700.00	28	2176.00
PAYABLE AMOUNT						9256.00

Commercial terms and conditions

1. Payment 80% advance along with PO balance before dispatch, 20%After installation.
2. Delivery period; 2weeks.
3. Tax :GST@18% for spares, 28%@Battery
4. Installation; Our scope.



Please arrange to release the PO at our above address

Bank name :HDFC Account no:50200082743176 IFSC Code:HDFC0004083

We hope you will find the above offer in line with our discussions and await your valuable order please free to call or mail us on above given number if any query.

Thank you, Sincerely,
BHAGATH MOHAN



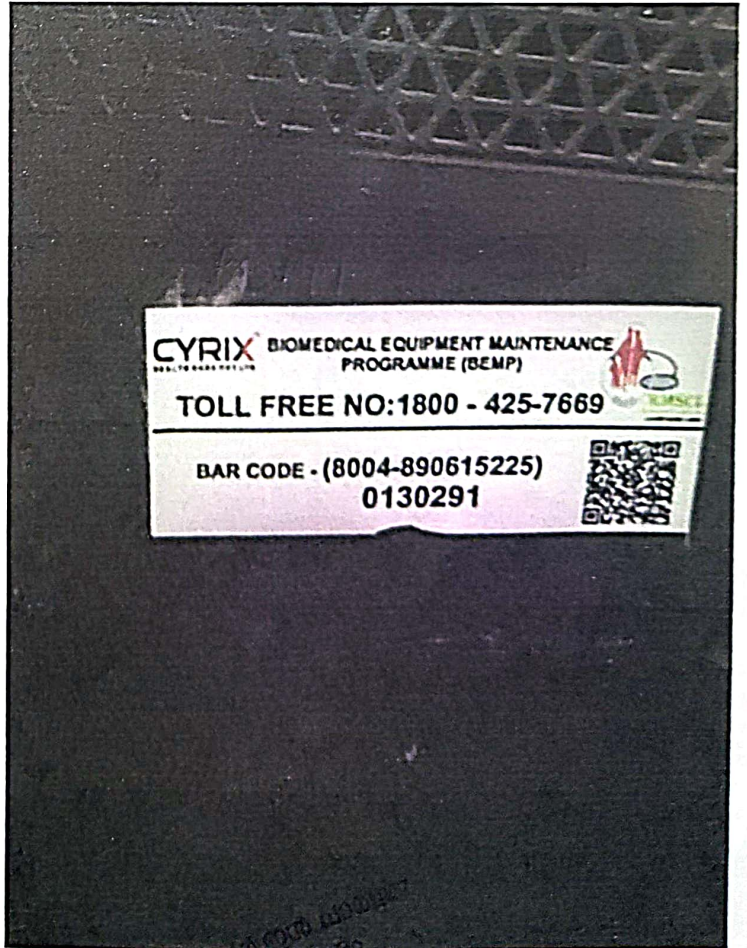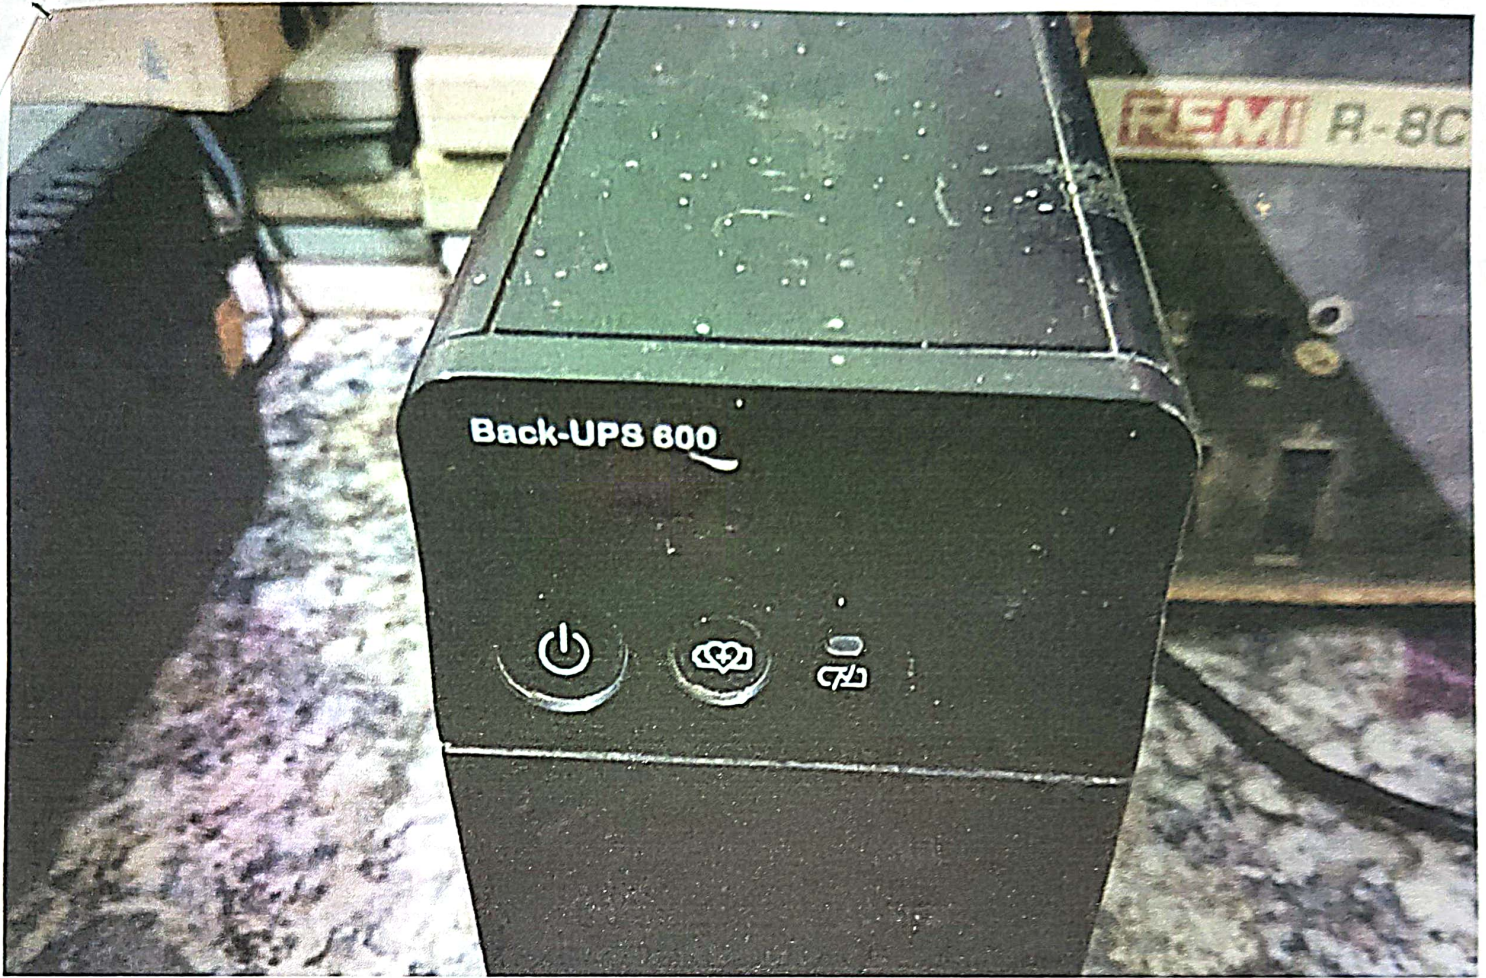

മെഡിക്കൽ ആവിരോധന പദ്ധതി
സാമൂഹ്യ ആരോഗ്യ കേന്ദ്രം
വുത്തന്തോപ്പ്, മിസ്സൂറി
സൗകര്യ വകുപ്പ്, മിസ്സൂറി



REGARDING QUOTATION FOR UPS-CHC ANCHUTENGU (0130192 0130178)

2 messages

Kasyep P V <kasyepcyrix@gmail.com>

Thu, 18 Jul 2024 at 10:02 pm

To: aionbackups12@gmail.com <aionbackups12@gmail.com>

Dear sir,

Kindly provide the service quotation for the 1 KV UPS at CHC Anchuthengu, Trivandrum

--

Thanks & Regards,

KASYEP PV

District Incharge , Trivandrum

CYRIX HEALTHCARE Pvt.Ltd

KLBEMP

Ph : +91 7593847134

kasyepcyrix@gmail.com

Bhagath Mohan <aionbackups12@gmail.com>

Thu, 18 Jul 2024 at 11:19 pm

To: Kasyep P V <kasyepcyrix@gmail.com>

Received your mail.

Thanks & Regards

Bhagath Mohan

PH:-8921950217

[Quoted text hidden]