



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

No : 125340

# CYRIX<sup>®</sup>

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

## Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala  
Ph : 98472 99500 Website :www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility: <i>Crit. Care &amp; Rehab Center</i>	Call Registration Date : ... <i>12.11.2024</i> .....
Address: ... <i>on road</i> .....	Caller ID : ... <i>146487</i> .....
Ph: ... <i>9495284102</i> .....	Date of Visit : ... <i>14.11.2024</i> .....
	Asset No : ... <i>0112186</i> .....
	EQPT Name : ... <i>rebulizer</i> .....
	Manufacture... <i>omron</i> ... Model : <i>NEE-el01</i>
	S. No... <i>2018081577</i> ... Dept... <i>OP</i> .....

Service Classification : Breakdown call  PMS  Calibration  Cust. Training

Problem Identified : ... *not working* .....

Action Taken : ... *checked and found no fuses from the unit. Identified resistor motor wear and piston defective. need to replace these. Spare for further checking and working condition of the equipment* .....

Completed  Date : ..... Time : ..... Spare Required


Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<i>Ajit George</i>	<i>14.11.2024</i>		

Customer Remark  Completed  Pending

Service Engineer Name : *Ajit*  
 Signature: *[Signature]*  
 Date: *14.11.2024*  
 Contact Number: *759284711*

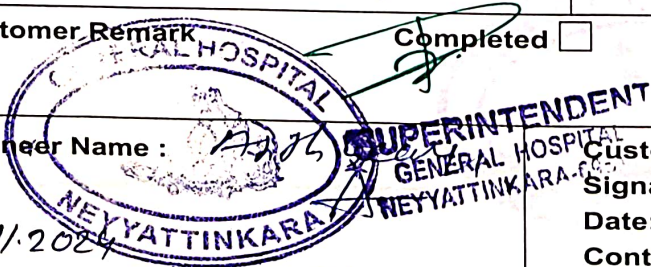


Customer Name : *SINDHU . B . H .*  
 Signature: *[Signature]*  
 Date: *14/11/2024*  
 Contact Number: *9447265614*  
 Designation : *Nursing Officer*  
 Hospital Seal



PROFORMA


RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)  
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

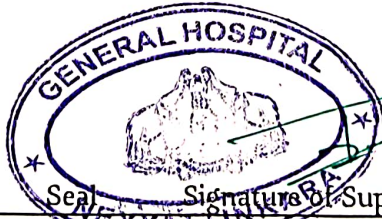Name of Hospital: GENERAL HOSPITAL NEYYATINKARA	Name of District: THIRUVANANTHAPURAM
Name of Equipment: NEBULIZER	Equipment ID & Barcode: 146437/0113186
Make: OMRON	Model: NE-C101
Serial Number: 20180815772VF	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: 03/10/2018	Present status of the equipment: Fully Damaged
Date of breakdown: 13/11/2024 (Date of registration of complaint through email/ Toll free)	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked and found no fumes from the unit. Identified nebulizer motor weak and piston defective. Need to replace these spares for further checking and working condition of the equipment.	
Recommendations for repair (required service details): Not recommending for repair.	
Cost of spares (specify parts and cost): NA	
# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 1353/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix Service report attached	
Reasons for recommending the equipment as BER: Checked and found nebulizer motor weak and piston defective. The unit was installed on 03/11/2018 and covered up to 6+ years. Quotation not attached since the spares are not available in the market. So recommending the unit for condemnation.	
<p>Kasyp.p.v <i>[Signature]</i> Name &amp; Signature of CYRIX Authority with date</p>	
Remarks of Junior Consultant (Biomedical) NHM: <p>Moton weak and piston damaged. So can be RBER.                      Complaint date : 13-11-2024                      Submission date . 27-12-2024</p>	
Recommended for BER (Yes/ No):	<p><i>[Signature]</i> MANEESHA MOHAN M.R.                      Junior Consultant (Biomedical)                      National Health Mission                      Thiruvananthapuram                      Signature of JC BM (NHM)</p>
Date: 31.12.2024	
<p>Date:  <i>[Signature]</i>                      Seal Signature of Superintendent                      SUPERINTENDENT                      GENERAL HOSPITAL                      NEYYATINKARA-695121                      Medical Officer (i/c)</p>	





Nebulizer

Date	Received from Stock	Received	Issued	Balance
19/3/12				1
23/3/2015	Received from stock (Dated page no 27)			1
17/6/2015	Inventori de cerul			1
5/8/2016	Received from stock			4
21/9/16	Received from stock			6
8/2/2017	Received from stock MSR page no: 28			6
16/10/17	Recd from stock (L.P)			9
	2 Nos. Condiemel as per order no 4920/17 dated 30/10/2017		2	7
10/4/18	Recd from stock (L.P)			9
3/10/18	Recd from stock unscripted Reg - 2			11
26/12/18	Portable Nebulizer Received from stock Invo. op su 5434/10 dated 26/12/18 Dash Health family welfare Society Bangalore by order no - DPM Su 74/18 dated 5/10/18	1		12
	(Stock) Stock Reg. No 4-5 pay	359		
29/5/19	Received from stock (Conscriptable - 3) As per order no. 48119 dated 1/2/2019 Nebulizer @ No Conscripted and received from Store.	3		14
	2 in unscriptable register -			12

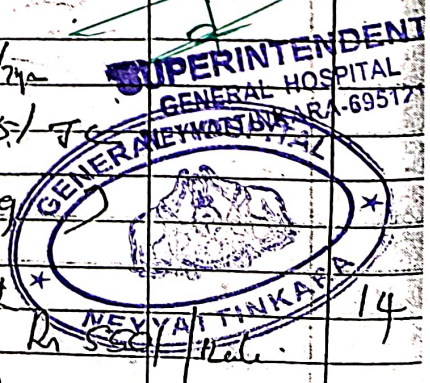

Balance (10) Page 11



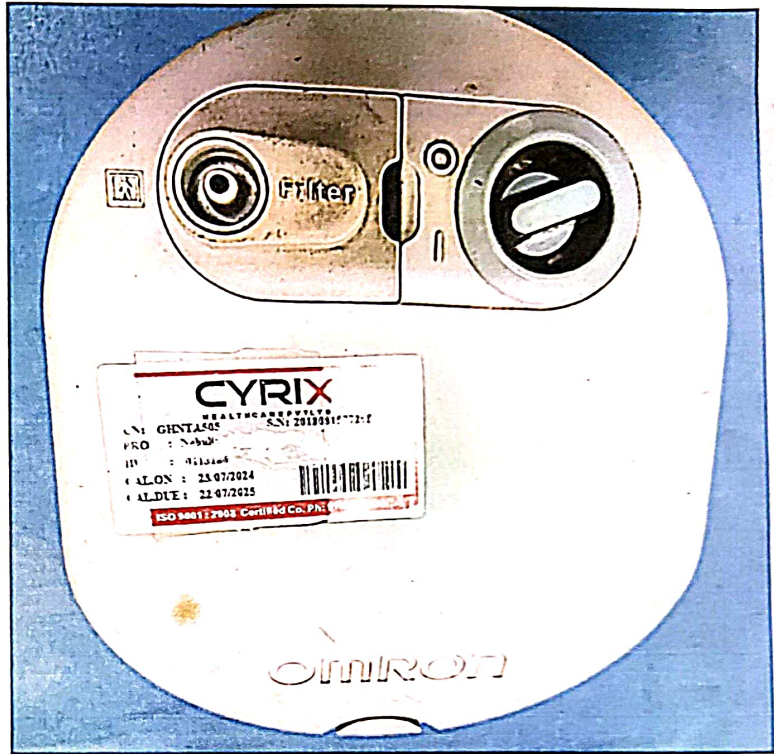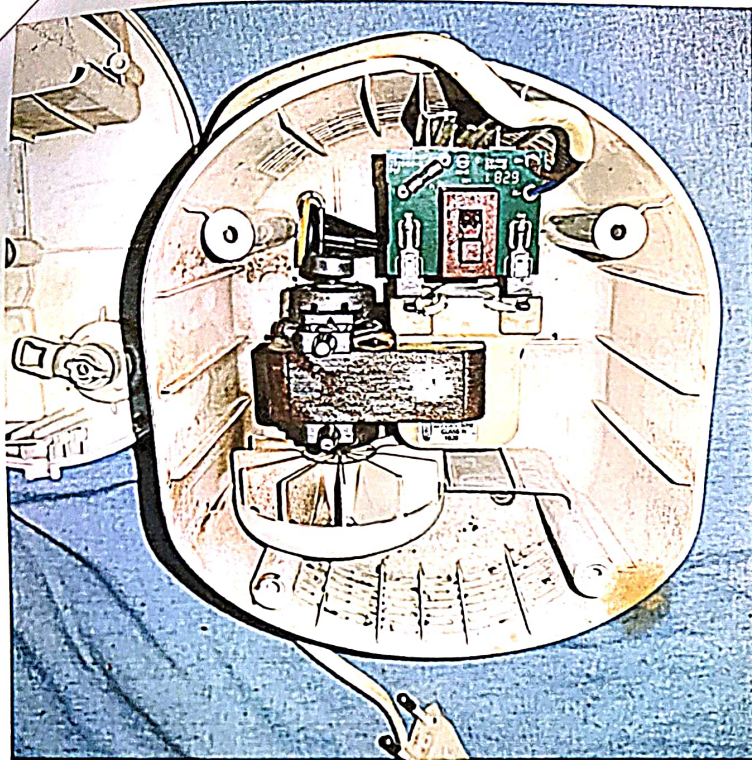


OMRON Compressor Nebulizer  
MODEL: NE-C101  
RATING: 230V ~ 50Hz 150VA

SN 2018081572VF  
OMRON HEALTHCARE Co. Ltd.  
KYOTO, JAPAN

EC REP  
OMRON HEALTHCARE EUROPE B.V.  
Scorplus 33, 2132 LR Hoofddorp,  
THE NETHERLANDS  
151a Pacific HQ: OMRON HEALTHCARE SINGAPORE PTE LTD.  
MADE IN VIETNAM

IP21  
CE 0197

QR CODE  
TOLL FREE NO: 1800 - 425-7669  
CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)  
BAR CODE - (8004-890615225)  
0113186

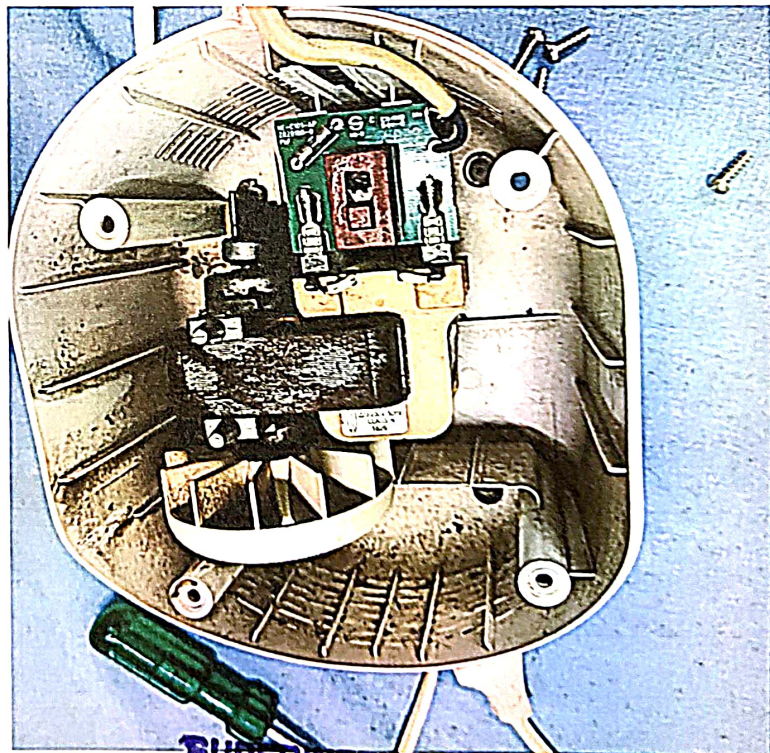

**SUPERINTENDENT**  
GENERAL HOSPITAL  
NEYYATTINKARA-695121

NEYYATTINKARA