


**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: PHC VALANCHERY	Name of District: MALAPPURAM
Name of Equipment: BIOCHEMISTRY ANALYSER	Equipment ID & Barcode: #149458-1040972
Make: ROBONIK	Model: PRIETEST TOUCH
Serial Number: AT4340413RBK	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: In Ticket master installation date is 23/06/2015, As per stock book installation date is 01/02/2015	Present status of the equipment: Fully damaged
Date of breakdown: 28/11/2024 Date of registration of complaint through email/Toll free): Toll free	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked the machine and found Primary board & display defective. Need to replace these spares for further checking	
Recommendations for repair (required service details): No recommendation	
Cost of spares (specify parts and cost): N/A	

#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: N/A	Asset Value: 64760/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report & OEM EOL Letter attached	

Reasons for recommending the equipment as BER: Checked the machine and found Primary board & display defective. In ticket master installation date is 23/06/2015, As per stock book installation date is 01/02/2015, Aged up to 9 years & 5 months. OEM informed that this machine is obsolete model, end of life letter issued. As per tender clause 5.3.14.2 We recommending the equipment for condemnation

10/12/2024 GJOKUL KT 
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
Verified with the damage of display and Primary board. AS per OEM the said model is obsolete

Recommended for BER (Yes/ No):
Date: 10/12/24



Signature of J.C. BM (NHM)
10/12/24
Jr. Consultant Biomedical Engineer
NHM Malappuram

Date: 12-12-24
*Not mandatory



Signature of Neema Venkatesh
12/12/24
Neema Venkatesh
Superintendent Medical Officer (i/c)
Attached Photograph

Seal //Based on the period of life and value as per the BER guidelines

Date: 06.12.2024

Dear Valued Customer,



Thank you for choosing **Robonik (India) Pvt. Ltd.** We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model: Prietest Touch) having **Serial No. AT4340413RBK.**

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT4340413RBK** as **End of Life (EOL) Notified.** (During from installation is 10 years).


Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK (INDIA) PVT. LTD.**

Authorised Signatory


12/12/24
മെഡിക്കൽ ഓഫീസർ
74X7 പ്രാഥമികാരോഗ്യ കേന്ദ്രം
വളാങ്ങാതി



ROBONIK (INDIA) PVT. LTD.

Plot No. 3 & 4, MOHIVALI MIDC, NEAR LADI NAKA, AMBERNATH (W) 421501, INDIA.
Telephone: +91 251-2689000 Website: www.robunikindia.in, Email: sales@robunikindia.com

< +91 98336 96980



wait few days Thursday

Ok 11:18 am

Howmach days 11:19 am

10 day s 11:19 am

Friday

Forwarded



File: 60.12.2021

Dear Valued Customer,

EOL Letter = Prietest Touch - AT4340413RBK.pdf

1 page • 89 kB • PDF

11:00 am

K 11:01 am

Saturday

This message was deleted

6:51 pm

Today

Hi 12:39 pm

Yes 12:40 pm



Message



Handwritten signature: Dr. Neeraj Kumar

Handwritten text: മെഡിക്കൽ ഓഫീസർ 74X7 പ്രാഥമികാരോഗ്യ കേന്ദ്രം വളാഞ്ചേരി

← +91 98336 96980



Thursday

PHC VALANCHERY
SEMI BIOCHEMISTRYANALYSER
TICKET ID =149558
BARCODE = 1040972
MAKE = ROBONIC
MODEL=PRITEST TOUCH
SERIAL NO=AT4340413RBK

11:07 am ✓✓

Missed voice call
Tap to call back 11:18 am

I am not in office 11:18 am

Wait few days 11:18 am

Ok 11:18 am ✓✓

Howmach days 11:19 am ✓✓

10 day s 11:19 am

Friday

⇒ Forwarded



Phone: 96.12.2631

Dear Valued Customer

Message



Handwritten signature
12/12/24
മെഡിക്കൽ ഓഫീസർ
24x7 പ്രാഥമികാരോഗ്യ കേന്ദ്രം
വളാഞ്ചേരി



1040972 biochemistry Abalyser PHC VALANCHERY Need price quotation for primary board & display

2 messages

Gokul K T <gokulcyrix@gmail.com>

Sat, 7 Dec, 2024 at 10:44 am

To: service@robonikindia.com

Cc: sanjana.support@robonikindia.com, Blesson Jose <Zm2.klbemp@cyrix.in>

Dear Sir, Madam

Can you send the Price quotation for Biochemistry analyser Primary board & Display , Make:Robonik , model :Prietest touch Sn:AT4340413RBK

Barcorde:1040972
Ticket id:149458
Biochemistry analyser
PHC VALANCHERY

GOKUL KT
CYRIX HEALTHCARE Pvt Ltd
DISTRICT INCHARGE
MALAPPURAM
9809314280


Gokul K T <gokulcyrix@gmail.com>

Wed, 11 Dec, 2024 at 12:42 pm

To: service@robonikindia.com

Cc: sanjana.support@robonikindia.com, Blesson Jose <Zm2.klbemp@cyrix.in>

Reminder
[Quoted text hidden]




Neema Venugopal
12/12/24
മെഡിക്കൽ ഓഫീസർ
24x7 പ്രാഥമികാരോഗ്യ കേന്ദ്രം
വളാഞ്ചേരി

SEMI AUTO ANALYSER (Robotic India Pvt. Ltd)
 Rintep scheme.

Date	From whom received To whom issued	Receipt	Issued	Balance	Sign	Remarks
01.1.2015	Transferring from page no: 110		Vol: IV			
			1	using		Omni
	Model : Pwetek Touch					
	Serial No.: AT430413R0K					
	Installation Date : 24-06-13					
	Accessories supplied					
	Power cord	1				
	Thermal paper roll	2				
	Paper roll rod	1				
	Dust cover	1				
	Tubing sheet	1				
	Stylus	3				
	Flow cell cleaning wires (feet)	1				
	Waste bottle	1				
	Sine wave UPS (30 break up)	1				
	Hallogen lamp	1				
	User manual	1				
	UPS - SNO : Owr 3041344					
	Model no : UPS 1 KVA					
	- ups taken for service on 25/10/16 - cond					
	replaced new one on 3/11/16					



12/12/24
 Dr. Neema Venugopal
 Scanned by CamScanner
 மதுரை மருத்துவ கல்வி
 மற்றும் மீன்வள அறிவியல்
 பல்கலைக்கழகம்

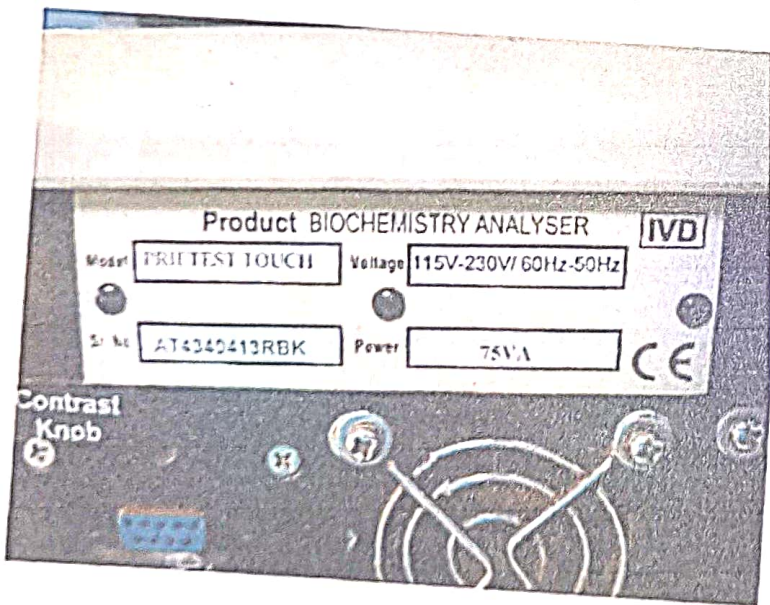

Dr. Neema Venugopal.
 മെഡിക്കൽ ഓഫീസർ
 2007 കോമിക്വാര്ട്ടർ ടി.എ.സി.
 തൃശ്ശൂർ