



**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: DH PERINTHALMANNA	Name of District: MALAPPURAM
Name of Equipment: CENTRIFUGE	Equipment ID & Barcode: #151262 - 1010034
Make: REMI	Model: R4C
Serial Number: NA	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: In ticket master installation date is 02-04-2015, As per stock book installation date is 22-04-2013	Present status of the equipment: Fully damaged
Date of breakdown: 07/12/2024 Date of registration of complaint through email/Toll free): Toll free	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Inspected the machine found Centrifuge Motor defective. Need to replace these centrifuge motor for further checking working condition of equipment.	
Recommendations for repair (required service details): No Recommendation	
Cost of spares (specify parts and cost): MOTOR : 6443/- TOTAL: 6443/-	
#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value:66 %	Asset Value: 9651/-
Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report attached & Oem Quotation attached.	

Reasons for recommending the equipment as BER: Checked the machine and found the motor defective. According to the ticket master, the installation date is 02/04/2015, whereas the stock book records the installation date as 22/04/2013. The equipment has aged 11 years and 7 months. The repair cost is 66% of the asset value, meeting both criteria for RBER. As per tender clause 5.3.14.1, we recommend the equipment for condemnation.



GROKUL K.T # 13/12/24
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
verified with the damage of motor. Machine is aged and is beyond economic repair

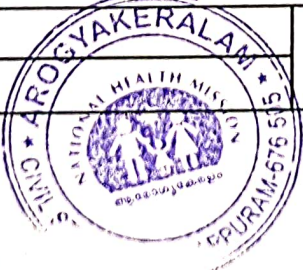Recommended for BER (Yes/ No):		 Signature of JC BM (NHM)
Date: 13/12/24		
Date:	Seal	Signature of Superintendent / Medical Officer (i/c)

Jr. Consultant Biomedical Engineer
NHM Malappuram

*Not mandatory #Based on the period of life and value as per the BER guidelines * Attach Photograph

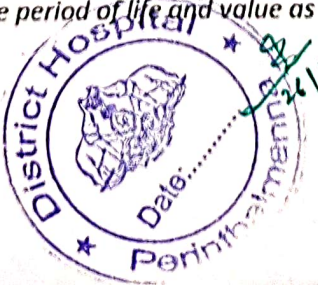

SUPERINTENDENT
 DISTRICT HOSPITAL
 PERINTHALMANNA-679 322
 MALAPPURAM DT.



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1004696

CYRIX[®]
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website :www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>DH</u>	Call Registration Date : <u>7/12/24</u>
Address..... <u>Perinthalmanna</u>	Caller ID : <u>151262</u>
..... <u>malappuram</u>	Date of Visit : <u>8/12/24</u>
Ph :	Asset No : <u>1010034</u>
	EQPT Name : <u>centrifuge</u>
	Manufacture..... <u>Remi</u> Model : <u>R-21C</u>
	S. No..... <u>na</u> Dept..... <u>LAB</u>

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : motor not working.....

Action Taken : checked the motor, found that motor damaged. need to replace these spare for further checking. necessary loads hrs of equipment.....

Completed Date : 8/12/24..... Time : 1:30pm..... Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>MOOKUL K-T</u>	<u>8/12/24</u>	<u>12:15pm</u>	<u>1:30pm</u>

Customer Remark Completed Pending

Service Engineer Name : <u>MOOKUL K-T</u>	Customer Name : <u>Ormadan-12</u>
Signature: <u>[Signature]</u>	Signature: <u>[Signature]</u>
Date: <u>8/12/24</u>	Date: <u>8/12/24</u>
Contact Number: <u>9809314080</u>	Contact Number: <u>9496443779</u>
	Designation : <u>SUPERINTENDENT</u>
	Hospital Seal

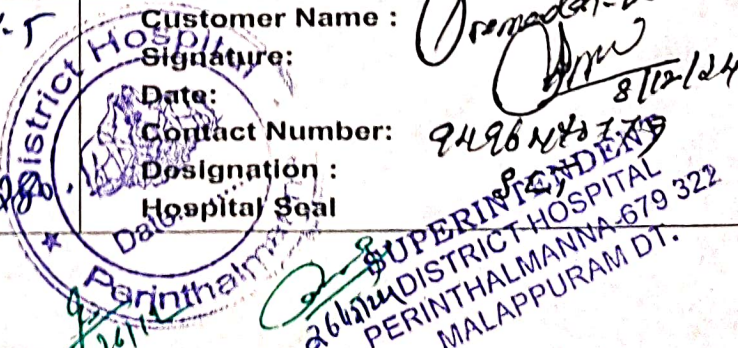

REMI SALES & ENGINEERING LIMITED



48/1103,Puthiyedath Road ,Vytilla P.O, Ernakulam Kochi-682019
Phone : 0484-682019,Mob: 8921409347 Email Id.:instservicekochi@remigroup.com/service@remilabworld.com

Corporate Off : Remi House, 3rd floor, 11 Cama Indl. Estate, Goregaon (East) Mumbai 400 063. INDIA
• Board: +91 22 4058 9888 SALES SUPPORT NO.8879448682• Email Id.: sales@remilabworld.com

QUOTATION CUM PROFORMA INVOICE

QN :DEC-20/24-25

Complaint No.		Customer Name & Address.:	Quotation No	PRINTED					
Dated	12/12/2024	DISTRICT HOPITAL	Date	12/12/2024					
ENGINEER NAME	vipin	PERINTHALMANNA	REF	Phone					
REF.	Phone	9809314280	DATE	12/12/2024					
Email	gokulcyrix@gmail.com	GOKUL KT							
Model no.	REMI: R-4C	SR NO. /MFG DT.	SLNO : 14517						
Sr No.	Description	Part code	HSN/SAC	Rate Rs.	Qty	Amount Rs. (A)	GST % (B)	GST Amt (C)	Total Amt (A+C)
	ELECTRIC MOTOR (RT)	ML25000140	850140	5460	1	5460	18%	983	6443
								TOTAL (D)	6443
	GAS CHARGING	0	0	0	0	0	18%	0	0
	SERVICE CHARGES		0	0		0	18%	0	0
								TOTAL (E)	6443
Rupees in Words:	Rs: Six thousand four hundred fourty three only								6443

Terms & Conditions:

- Spares are suitable only to use with REMI instruments & not for any other make.
- We will accept return of spares only if they are unused and not damage. At our discretion, the returned spare will be replaced. The difference in prices. If any will have to be borne by you.
- To ensure supply of correct spares, we suggest you to send us defective spare in advance with your request for which you want to purchase new spares.
- 100 % Advance along with your order confirmation
- Payment can be made by Cheque/ NEFT in our Bank account. For Cash Payment you must collect Receipt from recipient of cash failing which REMI will not be held responsible for any discrepancy.
- Courier/ transportation charges are payable at destination & not included in our price.
- Validity. The quotation is valid for 30 days from the date of this quotation / Proforma Invoice
- Subject to Ernakulam Jurisdiction only

REMARKS : PAYMENT 100% ADVANCE

For REMI SALES & ENGINEERING LTD



BANK DETAILS FOR REMI SALES & ENGINEERING LTD.

- | | | |
|---------------------------|----------------------------------|-------------------------------|
| • A/C NO: 35699154671 | • Bank Name: STATE BANK OF INDIA | • BRANCH: ELAMAKKARA |
| • IFS CODE: SBIN0013223 | • MICR CODE:682002053 | • SWIFT CODE: SBININBB395 |
| • GST NO: 32AAACR0421M1Z5 | • PAN NO: AAACR0421M | • CIN NO. U31100MH198PL022314 |



PRICE ENQUIRY 1010034 CENTRIFUGE @ DH PPERINTHALMANNA -MALAPURAM
(Ticket id 151262)

4 messages

Gokul K T <gokulcyrix@gmail.com>
To: instservicekochi@remigroup.com
Cc: Blesson Jose <Zm2.klbemp@cyrix.in>

Tue, 10 Dec, 2024 at 6:03 pm

Dear sir,

There is a complaint reported from DH PERINTHALMANNA - MALAPURAM, Regarding the complaint with Centrifuge Remi , R4C, serial Number - 14517, barcode number (1010034). Required price quotation for following spares, kindly share the estimate.

●MOTOR

GOKUL KT
CYRIX HEALTHACARE
DISTRICT INCHARGE
MALAPPURAM
9809314280

Gokul K T <gokulcyrix@gmail.com>
To: instservicekochi@remigroup.com
Cc: Blesson Jose <Zm2.klbemp@cyrix.in>

Wed, 11 Dec, 2024 at 2:59 pm

Reminder
[Quoted text hidden]

Gokul K T <gokulcyrix@gmail.com>
To: instservicekochi@remigroup.com
Cc: Blesson Jose <Zm2.klbemp@cyrix.in>

Thu, 12 Dec, 2024 at 12:27 pm

Remider
[Quoted text hidden]

instservicekochi <instservicekochi@remigroup.com>
To: Gokul K T <gokulcyrix@gmail.com>
Cc: Blesson Jose <zm2.klbemp@cyrix.in>, REMI Group - Kochi - Vishnu S K <kochisales.hcd@remigroup.com>, kochi@remigroup.com

Thu, 12 Dec, 2024 at 12:59 pm

Dear Sir,

Please find the attached PROFORMA INVOICE for your reference. **PLEASE RELEASE THE PAYMENT IN ADVANCE.**

Regards

REMI KOCHI


INST DIV.

Govt: Hospital, Perinthalmanna



STOCK REGISTER OF LABORATORY

Name of Articles ELECTRIC CENTRIFUGE


Date	No and date of Voucher or Invoice	From whom received of whom issued	Receipt	Issued	Balance	Initials of receiver	Remarks
7.6.2010	29.10.90	B.F. from old stock book (1)	03		03	JS 7/6/2010	EDAs: CE 1
	24.6.92 (UNICEF)	Page no: 6					CE 2 CE 3
	30.5.2001	[LAB DIAGNOSTIC] CAT I					
		Condemned as per order NO: A3/1300/2011 dt 24.01.2012					
		Supdt. THRH Perinthalmanna →	2	01		JS	Remi General
22.4.2013		From store.	1	2		JS	Purpos Lab Centrifuge model R-4c with Swingout Head R-41 capacity (x15ml)
		Unit Price 15000.00 Net value 15000.00 Tax 5.011 Total 15750.00					Using in the lab.
6.11.2013		Centrifuge From Store model Remi (1)	1	3		JS	R 20776 R 215540 Tax 1145000 26109.00
		8x15ml Swingout Head (1)					
		Using in the lab.					
8.5.14		Remi R-8 CD X Deluxe Laboratory Centrifuge (1)	1	4			26200 4030 1261.50 <u>26492.1</u>
		R 81 - Remi 16x15 ml Swing out Head (1)					
		code no: (414)67 (254)10 (21)0696					
		Using in the lab.					

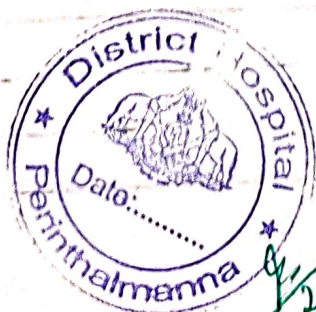

8/5 to page 07
SUPERINTENDENT
 DISTRICT HOSPITAL
 PERINTHALMANNA-679 322
 MALAPPURAM DISTRICT
 (CCM)

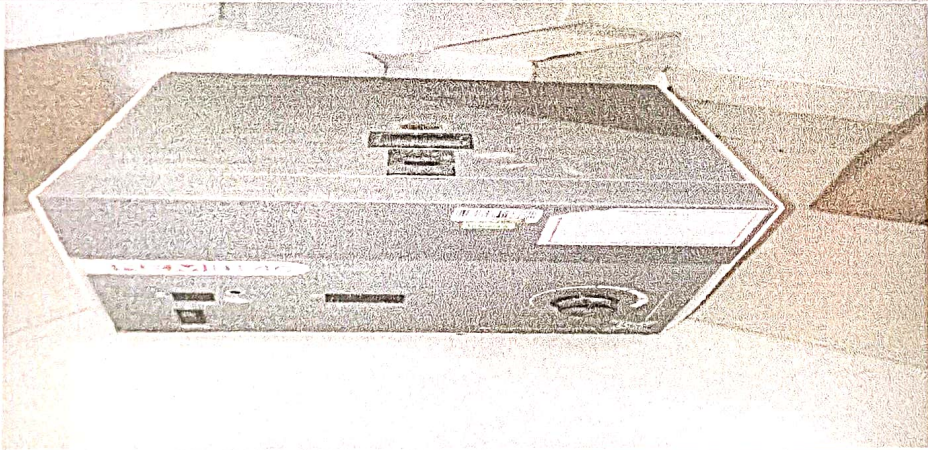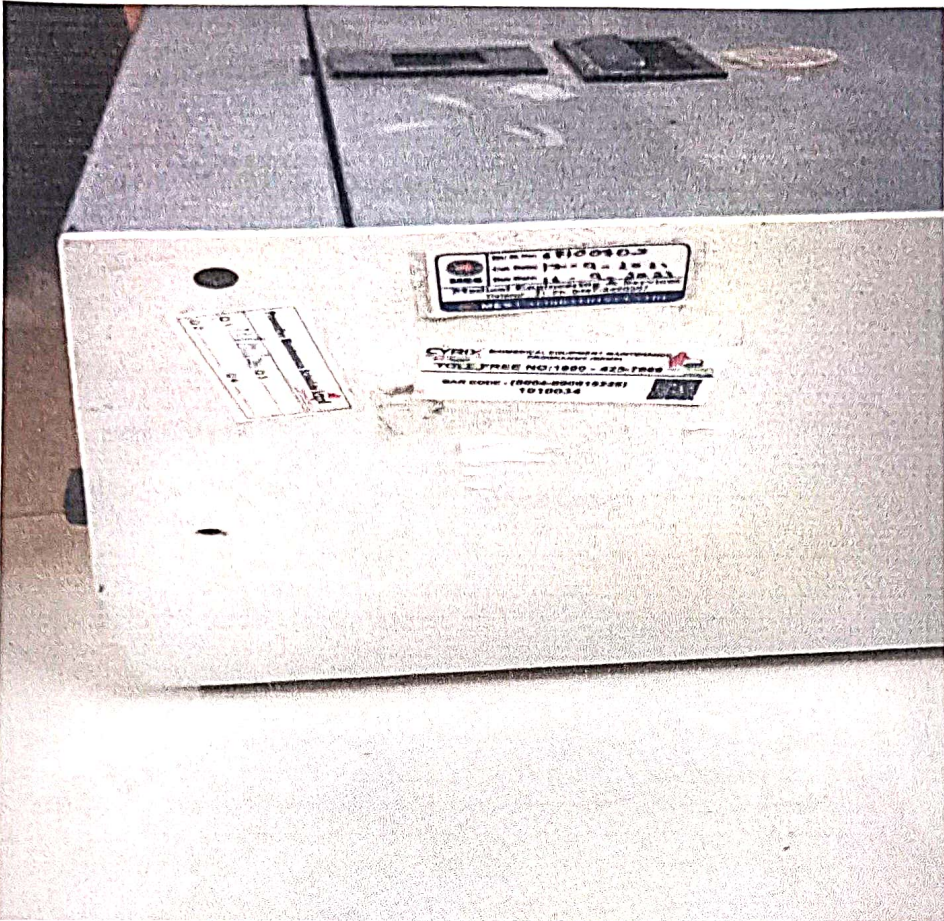

Handwritten signature and date:
26/11/24

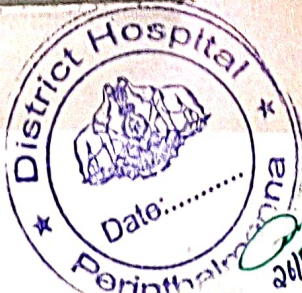

Handwritten date and signature: 26/11/24
**SUPERINTENDENT
DISTRICT HOSPITAL
PERINTHALMANNA-679 322
MALAPPURAM DT.**