

**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: UPHC KARIYAD	Name of District: KANNUR
Name of Equipment: DRY BATH INCUBATOR	Equipment ID & Barcode: #141879 – 1341220
Make: EURO	Model: ELECTRA
Serial Number: N/A	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: In ticket master installation date is 27/01/2020, As per the stock book installation date is 08-06-2020 (stock book attached for reference)	Present status of the equipment: Fully damaged
Date of breakdown: 21/10/2024 Date of registration of complaint through email/Toll free): Toll free	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked the dry bath incubator and found control board defective, need to be replace this spare for further checking of machine.	
Recommendations for repair (required service details): No recommendations	
Cost of spares (specify parts and cost): NA	

#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: NA	Asset Value: 21500/-
-------------------------------------------------------------------------------------------	----------------------


Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix Service report attached EOL attached.

Reasons for recommending the equipment as BER: Checked the dry bath incubator and found control board defective, need to be replace this spare for further checking of machine. In ticket master installation date is 27-01-2020, As per the stock book installation date is 08-06-2020 aged up to 4 years and 5 months. OEM informed that this model is obsolete. End of life letter issued. As per tender clause 5.3.14.2 we recommending the equipment for condemnation.


Rasilraj Rasilar

Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM: *Checked and identified that machine not working due the defective the control board, and the OEM informed it is an obsolete model. Aged up to 4 years and above. So recommended for BER as per BER protocol.*

Recommended for BER (Yes/ No): <i>Yes</i>	
Date: <i>11/12/24</i>	

Date:	Seal	Signature of Superintendent / Medical Officer (i/c)
-------	------	-----------------------------------------------------



[Signature]

*Not mandatory

#Based on the period of life and value as per the BER guidelines



MEDCO HEALTHCARE
1ST Floor ME complex Airport Road,
Mundayad Kannur, 670594

28/11/2024

To,

M/s CYRIX HEALTH CARE
First Floor, Petta Junction 301647 B
Poonithura, Ernakulam - 682038

Sub: Reg. End of Life of an DRY BATH INCUBATOR

Dear Sir/Madam,

We would like to inform you that the equipment as per the below details is very old and the spare parts are not available. Hence we are unable to repair the equipment.

Equipment: Dry bath Incubator

Model : ELECTRA

SN:

MAKE: EURO

Thanking you

Akshay.M.P



Manager
Medco Healthcare



1ST Floor ME complex Airport Road,
Mundayad Kannur, 670594



medcohealthcarekn@gmail.com
+91 7560901848

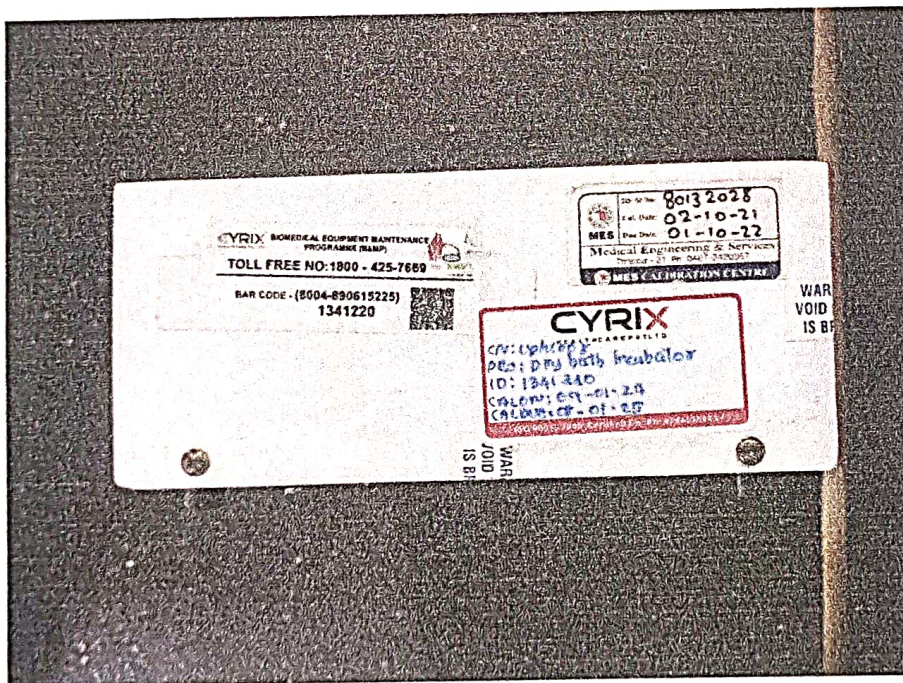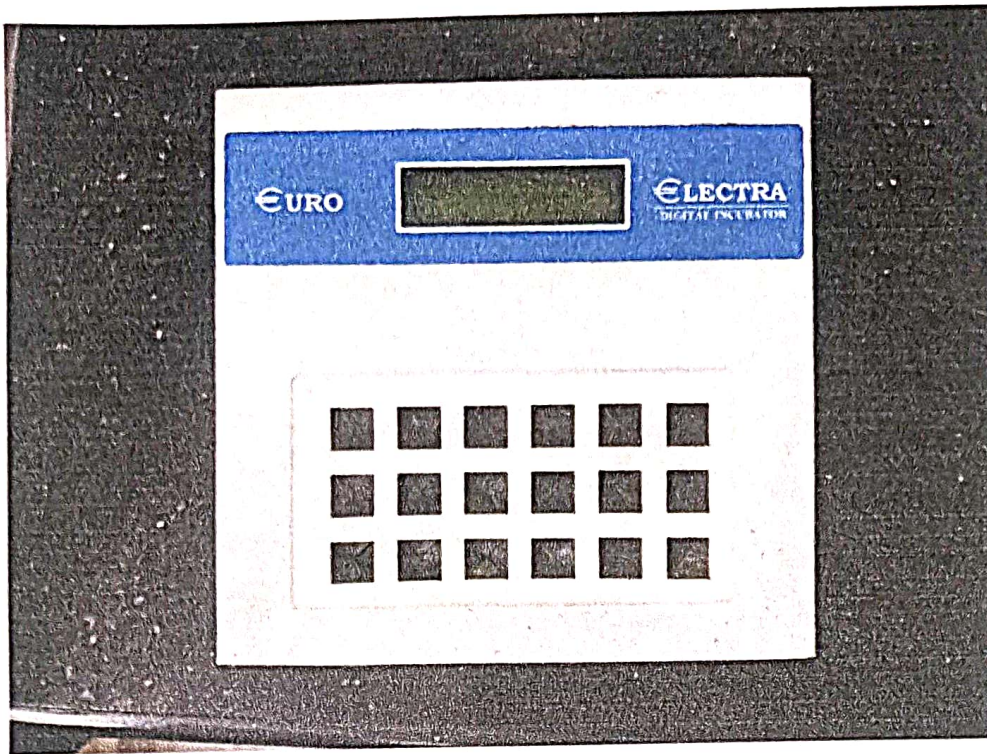

MEDICAL OFFICER
UPHC - PANOOR

