

PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: THQH MALAPPURAM	Name of District: MALAPPURAM
Name of Equipment: ULTRASOUND MACHINE	Equipment ID & Barcode: #150997-1021715
Make: ALOKA	Model: PROSOUND 4
Serial Number: M00181C	Warranty details: No Warranty
Date of purchase/Year of manufacture/Installation Date: In Ticket master installation date is 05/05/2010, Actual installation date As per stock book is 23/07/2010	Present status of the equipment: Fully damaged
Date of breakdown: 06/12/2024 Date of registration of complaint through email/Toll free: Toll free	*AMC/CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Checked the machine and found Main board & display defective. Need to replace these spares for further checking working condition of machine.	
Recommendations for repair (required service details): No recommendation	
Cost of spares (specify parts and cost): N/A	
#Percentage value of the cost of spares with respect to Cost of Purchase/Asset Value: N/A	Asset Value: 4,84,441/-


Abstract of Service Report provided by the OEM/Authorized Service Provider/CYRIX (Attached or Not): Cyrix service report & OEM EOL Letter attached

Reasons for recommending the equipment as BER: The machine was inspected and found to have a defective mainboard and display. The installation date is recorded as 05/05/2010 in the Ticket Master and 23/07/2010 in the Stock Book, making the equipment 14 years and 7 months old. The OEM has confirmed that this is an obsolete model, and an End of Life (EOL) letter has been issued. As per tender clause 5.3.14.2, we recommend the equipment for condemnation.

GOKUL K T # 17/12/24
 Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
 Verified with the damage of Main board & Display. As per OEM, the said model is obsolete. Beyond economic repair.

Recommended for BER (Yes/No):
 Date: 17/12/24

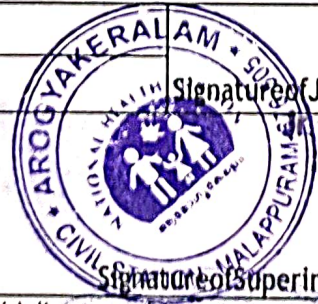

Signature of JCBM (NHM)
 Consultant Biomedical Engineer
 NHM Malappuram
 17/12/24

Date: 20/12/24 Seal Signature of Superintendent/Medical Officer (I/c) 16/12/24

andatory Based on the period of life and value as per the BER guidelines Attach Photograph
 SUPERINTENDENT
 TALUK HEAD QUARTERS HOSPITAL
 MALAPPURAM



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1023657



ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website :www.cyrix.com | Email : bemp.kl@cyrix.in

<p>Health Facility: <u>JHBM</u>.....</p> <p>Address: <u>MALAPPURAM</u>.....</p> <p><u>MALAPPURAM (DISTRICT)</u></p> <p>Ph:</p>	<p>Call Registration Date : <u>06/12/2024</u>.....</p> <p>Caller ID : <u>150997</u>.....</p> <p>Date of Visit : <u>07/12/2024</u>.....</p> <p>Asset No : <u>1021715</u>.....</p> <p>EQPT Name : <u>ULTRASOUND MACHINE</u></p> <p>Manufacture: <u>ALOKA</u>... Model : <u>PROSOUND 4</u></p> <p>S. No. <u>MO0181C</u>..... Dept: <u>LABOUR ROOM</u></p>
--	--

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : ultra sound machine not working.

Action Taken : checked the machine and found main board & display defective. Need to replace these spares for further checking working condition of machine.

Completed Date : 7/12/24 Time : 11:30 AM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrux Engineer	Date	Start Time	End Time
<u>Shihobudhnan</u>	<u>7/12/24</u>	<u>10 AM</u>	<u>11:30 AM</u>

Customer Remark Completed


SUPERINTENDENT
TALUK HEAD QUARTERS HOSPITAL
MALAPPURAM

Service Engineer Name : Shihobudhnan
 Signature: [Signature]
 Date: 7/12/2024
 Contact Number: 9072522046

Customer Name : Jodu's
 Signature: [Signature]
 Date: 7/12/2024
 Contact Number: 9526781507
 Designation : SNO
 Hospital Seal

Announcement on spare parts supply deadline

Date August 10th, 2023

Ref No. GSD_23-018

Dear Partners,

We would like to inform you that service parts for Prosound 2, Prosound 4 and Prosound 6 are discontinued because of these models have been passed seven(7) years since the shipment from Japan.

1. Latest shipment date from the Japan factory to India

- Prosound 2: August 2010
- Prosound 4: December 2012
- Prosound 6: October 2008

2. Spare parts supply deadline

seven (7) years since each shipment from Japan

Sincerely yours,



Takayuki Tawara
Manager
Service Solution Group, US Business Operation Division,
Ultrasound Diagnostic Systems Division,
FUJIFILM Healthcare Corporation



EOL for ALOKA PRESOUND

2 messages

Assistant Manager Purchase <ampurchase@cyrix.in>

Thu, 10 Aug 2023 at 3:58 pm

To: msantosh@trivitron.com <msantosh@trivitron.com>

Cc: Cyrix Purchase Mgr. <purchasemgr@cyrix.in>, Aneesh Kottiyoor <aneeshcyrix@gmail.com>, Blessen Jose <bleseencyrix@gmail.com>, Project Manager KLBEMP <pm.bempkl@cyrix.in>

Santhosh sir,

As per the discussions we had, please share the EOL letter for Aloka Presound 4 Ultrasound Machine, Sr No.M00196C

Thanks & Regards

Smija James K

Assistant Manager - Purchase

PH No: 9072522067

ampurchase@cyrix.in

smijacyrix@gmail.com

www.cyrixhealthcare.com

Cyrix Healthcare Pvt Ltd

| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India

KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH

SANTOSH MARATHI <msantosh@trivitron.com>

Thu, 10 Aug 2023 at 5:31 pm

To: Assistant Manager Purchase <ampurchase@cyrix.in>

Cc: Cyrix Purchase Mgr. <purchasemgr@cyrix.in>, Aneesh Kottiyoor <aneeshcyrix@gmail.com>, Blessen Jose <bleseencyrix@gmail.com>, Project Manager KLBEMP <pm.bempkl@cyrix.in>

Dear Smija,

Please find attached end of Spare part support letter. This is applicable for all the serial numbers of said models.

Thanks And Regards

Santosh Marathi

Technical Manager


M : +91 9731681153/ 7259021323

Trivitron Healthcare Pvt. Ltd. 801/802, Shelton Cubix, 8th

Floor Plot No.87,Sector-15, CBD Belapur Navi Mumbai -

400614, India

TRIVITRON
HEALTHCARE
speaking your language


 WE ARE
GREAT PLACE TO WORK - CERTIFIED™
Building and sustaining High-Trust, High-Performance Culture™

Error! Hyperlink reference not valid.

Customer Care +91 98400 80008



ULTRA SOUND SCANNER.

	Barcode → 1021715		
23/7/2010	Rd from the store		
	Rs 8,51,000/-	1	1
	Convex Probe		
	T.V Probe		
	DVD Recorder		
	Thermal Printer		
	U PS. (Main Stock Register Page no	210	VOI III A. O
	Ph No: 0484-3258117		
	" 0422-3259212		
	" 8754426617		
	(Prasound-H-Aloka) Company		
	NIBIN-8136888509 (Cochin)		
	Manj - 08129803685, 08129803586		
	Barcode → 1021715		
	Greeshma Bio Medical	94965	9937
	Engineer		
1/2/22	Rd from the store		
	(Portable Ultrasound machine	1	2
	- Trolley + probes	1	
	probes (Adult + paediatric)	3	
	Treat to Instruments & Equipment Register		
	Vol III Page - 61	2	2

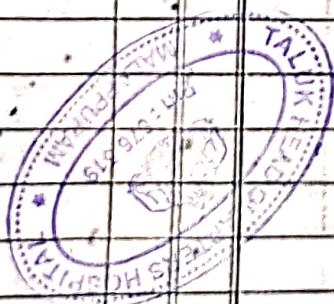

[Handwritten signature]
26/1/22

SUPERINTENDENT
TALUK HEAD QUARTERS HOSPITAL
MALAPPURAM

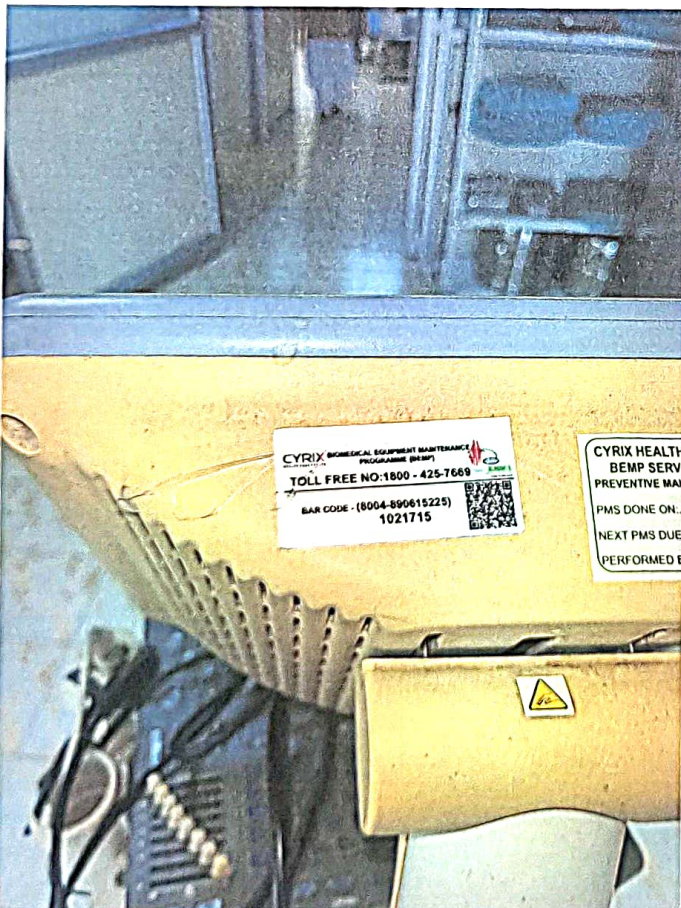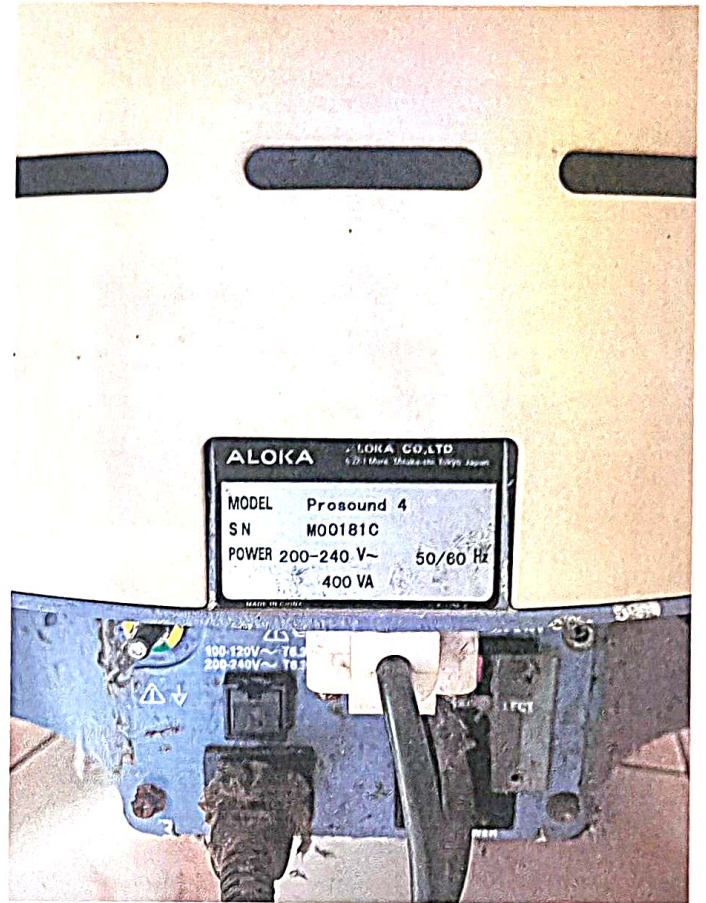

[Handwritten signature]

SUPERINTENDENT
TALUK HEAD QUARTERS HOSPITAL
MALAPPURAM

