

**PROFORMA**  
**RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)**  
**BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Name of Hospital: GRD NGO QUATTERS	Name of District: KOZHICODE
Name of Equipment: WEIGHING MACHINE	Equipment ID & Barcode: 152164 & 1140418
Make: SAMSO	Model: NA
Serial Number: NA	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: In ticket master installation date is 10/06/2019, Actual installation date As per stock book is 30/06/2019	Present status of the equipment: Fully damaged
Date of breakdown: 12/12/2024	*AMC/ CAMC Period agreed
Date of registration of complaint through email/Toll free): Toll free	at the time of purchase: No AMC/CAMC
Action taken: Checked and found front case, main board and load cell defective. Need to replace these spares for further checking of working condition of the equipment.	
Recommendations for repair (required service details): Not recommending for repair	
Cost of spares (specify parts and cost): N/A	

#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: N/A	Asset Value: 1600 /-
--	----------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report attached

Reasons for recommending the equipment as BER: Checked and found front case, main board and load cell defective. Need to replace these spares for further checking of working condition of the equipment. In ticket master installation date is 10/06/2019, as per stock book installation date is 30/06/2019 (stock book attached for reference) Equipment out lived 5 Years 5 Month, with an asset cost of rupees 1600. Quotation not submitted since spares are not available in the market So we recommend the equipment for condemnation.

JINEESH PP *Jineesh*  
 Name & Signature of CYRIX Authority with date 17/12/2024

Remarks of Junior Consultant (Biomedical) NHM:  
*checked & found that front case, main board and load cell defective. Machine installed on 30/06/2019. Spares are not available in the market. So recommended for condemnation.*

Recommended for BER (Yes/ No): Yes <input checked="" type="checkbox"/>	Consultant Bio Medical Engineer National Health Mission Kozhikode
Date: 17/12/2024	Signature of JC BM (NHM)

Date: 18/12/2024	Seal <b>Medical Officer</b> <b>G.R.D., N.G.O. Quarters</b> <b>Vellimadukuru</b>	Signature of Superintendent / Medical Officer (i/c)
------------------	--	---

\*Not mandatory      #Based on the period of life and value as per the BER guidelines      \* Attach Photograph





# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

No : 130257

## CYRIX<sup>®</sup>

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>GIRD N.G.O. Quarters</u> Address..... <u>Kozhikode</u> Ph :..... <u>8130802658</u>	Call Registration Date : .. <u>12/12/24</u> ..... Caller ID : ..... <u>152164</u> ..... Date of Visit : .. <u>13/12/24</u> ..... Asset No : ..... <u>1140418</u> ..... EQPT Name : .. <u>weighing Machine</u> ..... Manufacture.. <u>SAMSUNG</u> ... Model : .. <u>NA</u> ..... S. No..... <u>NA</u> ..... Dept..... <u>OP</u> .....
--	--

Service Classification : Breakdown call  PMS  Calibration  Cust. Training

Problem Identified : ..Not switching on.....

Action Taken : ..checked and found that front case physically damaged, main board and load sensor defective. need to replace these spares for further checking of working condition of the equipment.....

Completed  Date : ..13/12/24.. Time : ..11:50 am.. Spare Required


Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			



Cyrix Engineer <u>Mubashir</u>	Date <u>13/12/24</u>	Start Time <u>11:10 am</u>	End Time <u>11:50 am</u>
-----------------------------------	-------------------------	-------------------------------	-----------------------------

Customer Remark Completed  Pending

Service Engineer Name : <u>Mubashir</u> Signature: <u>[Signature]</u> Date: <u>13/12/24</u> Contact Number: <u>7593847163</u>	Customer Name : <u>GIRD Vellimadukunnu</u> Signature: <u>[Signature]</u> Date: <u>13/12/24</u> Contact Number: <u>9446061155</u> Designation : <u>Pharmacy</u> Hospital Seal: <u>[Seal]</u>
--	--

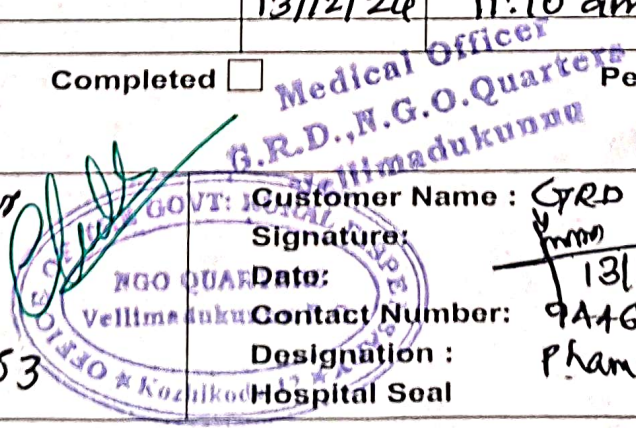



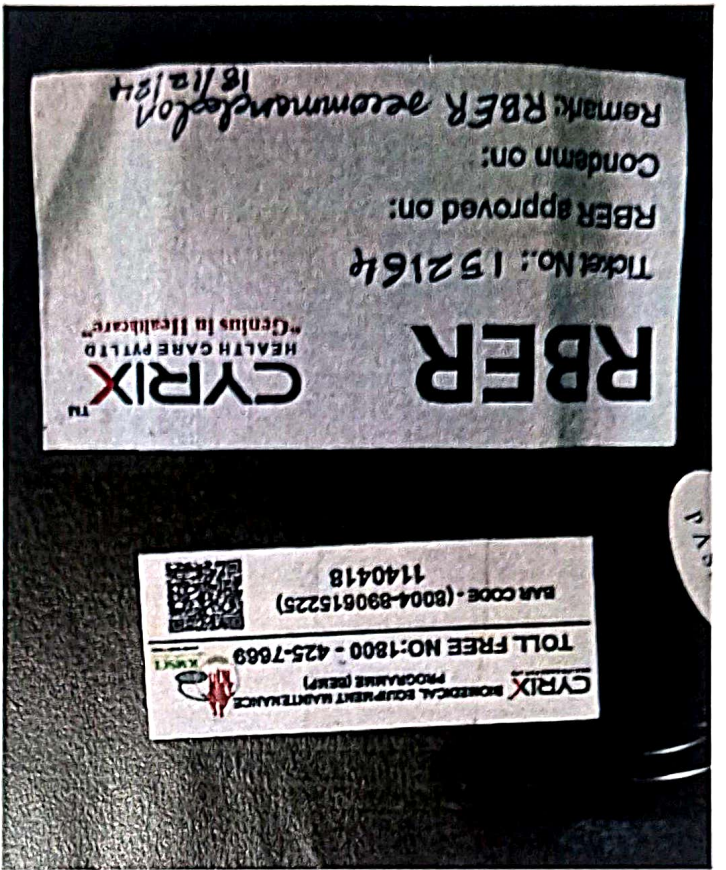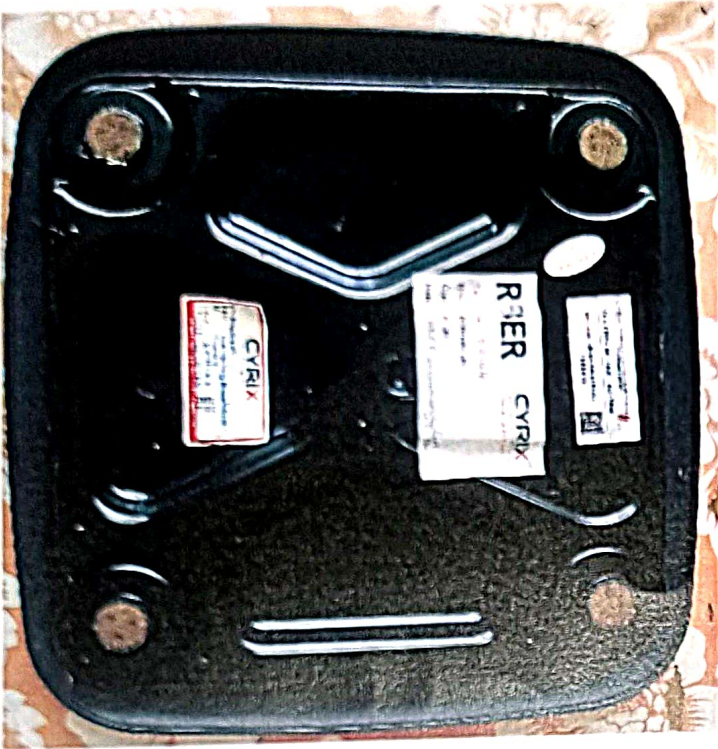

Medical Officer  
R.D., N.G.O. Quarters  
Vellimadukku

*[Handwritten signature]*  
16/12/24