

PROFORMA

RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)  
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: GH KASARGOD	Name of District: KASARGOD
Name of Equipment: NEBULISER	Equipment ID & Barcode: 152105, 1411269
Make: LIFE LINE	Model: ALPHA
Serial Number: N/A	Warranty details: No Warranty
Date of purchase/ Year of manufacture/ Installation Date: In ticket master installation date is 19/05/2015. Actual installation date As per stock register is 19/12/17	Present status of the equipment: Fully damaged
Date of breakdown: 11/12/2024	*AMC/ CAMC Period agreed
Date of registration of complaint through email/Toll free): Toll free	at the time of purchase: No AMC/CAMC
Action taken: Inspected the machine and found that Machine has no fumes out, upon further checking, found nebulizer motor with piston are defective. Need to replace these spares for further checking working condition of machine.	
Recommendations for repair (required service details): Not recommending for repair	

Cost of spares (specify parts and cost): N/A

#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: N/A	Asset Value: 1353
--	-------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report attached.

Reasons for recommending the equipment as BER: Upon inspection, it was found that the machine has no fumes output, and both the motor and piston are defective. According to Ticket Master, the installation date is 19/05/2015, while the stock register indicates the installation date as 19/12/2017, with an asset cost of ₹1,353. A quotation was not submitted as the required spares are unavailable in the market. Therefore, we recommend condemning the equipment..

Ajit Babbar  
17/12/24  
Name & Signature of CYRIX Authority with date


Remarks of Junior Consultant (Biomedical) NHM: checked and identified that machine not working due to the motor and piston are defective. Aged up to 7 years and above. spare quotation not submitted. But the spare cost economically not feasible. So recommend for BER as per BER Protocol.

Recommended for BER (Yes/ No): yes.	Signature of JC BM (NHM) 17/12/2024
Date: 17/12/2024	

Date: \_\_\_\_\_ Signature of Superintendent / Medical Officer (i/c)

\*Not mandatory

Based on the period of life and value as per the BER guidelines

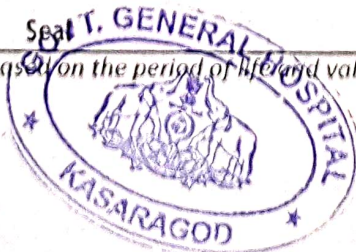

Signature of Superintendent / Medical Officer (i/c)  
Smt. General Hospital  
KASARGOD  
(P.O.) KASARGOD - 671121



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

No : 139124

**CYRIX**<sup>®</sup>  
HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

Health Facility..... <u>GH Kasaragod</u> .....	Call Registration Date : <u>11-12-24</u> .....
Address..... <u>Kasaragod</u> .....	Caller ID : <u>152105</u> .....
..... <u>Kerala</u> .....	Date of Visit : <u>12-12-24</u> .....
Ph: <u>9745374128</u> .....	Asset No : <u>1411269</u> .....
	EQPT Name : <u>nebulizer</u> .....
	Manufacture <u>life line</u> Model : <u>Alpha</u> .....
	S. No. <u>AA</u> Dept. <u>Laboratory</u> .....

Service Classification : Breakdown call  PMS  Calibration  Cust. Training

Problem Identified : motor, piston issues

Action Taken : checked the machine and found problem with motor and piston, need to replace those spare parts checked working condition of the equipment

Completed  Date : 12-12-24 Time : 10:40 Am Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Ajith Babu K</u>	<u>12-12-24</u>	<u>10:00 AM</u>	<u>10:40 AM</u>


Customer Remark  Completed  Pending

Service Engineer Name : Ajith Babu K Customer Name : SUSHAMA  
 Signature: [Signature] Signature: [Signature]  
 Date: 12-12-24 Date: 12/12/24  
 Contact Number: 8846079288 Contact Number: 9745374128  
 Designation : SNO Designation : Superintendent  
 Hospital Seal



[Signature]  
SUPERINTENDENT  
GOVT. GENERAL HOSPITAL  
KASARAGOD  
KASARAGOD - 686001



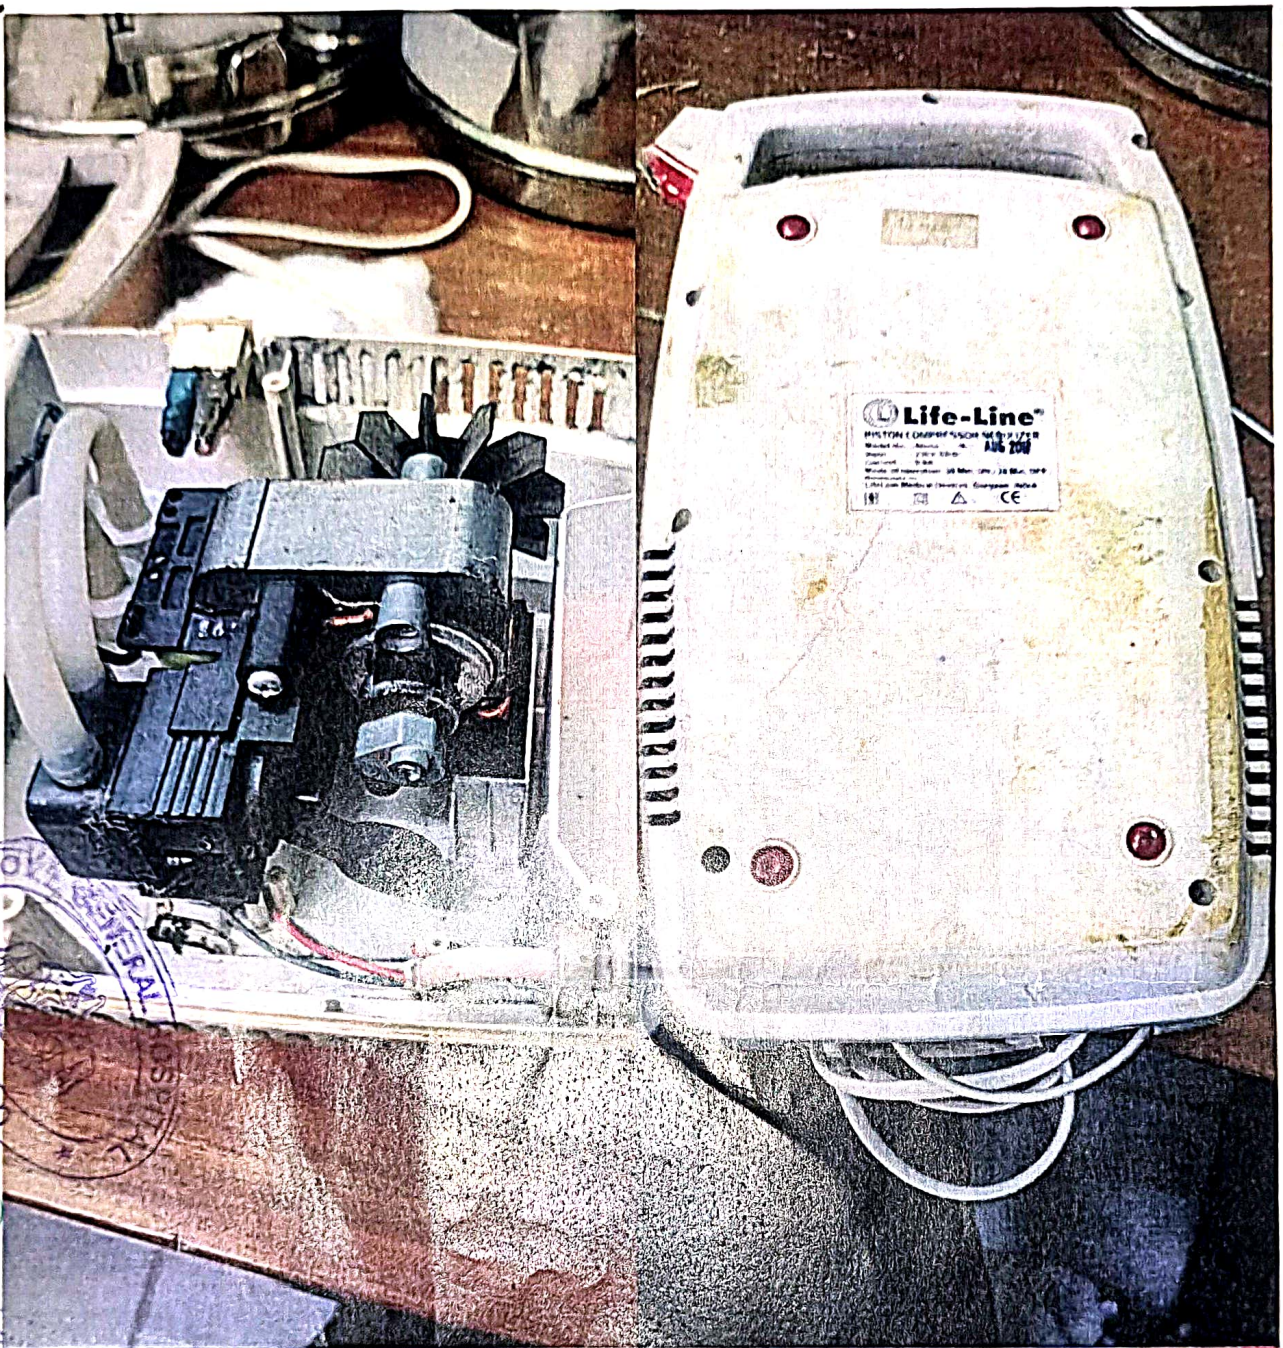

GOVT. GENERAL  
KASARAGOD  
SISTEM

GOVT. GR  
(P.O.)

